

FIG. 1

2/47

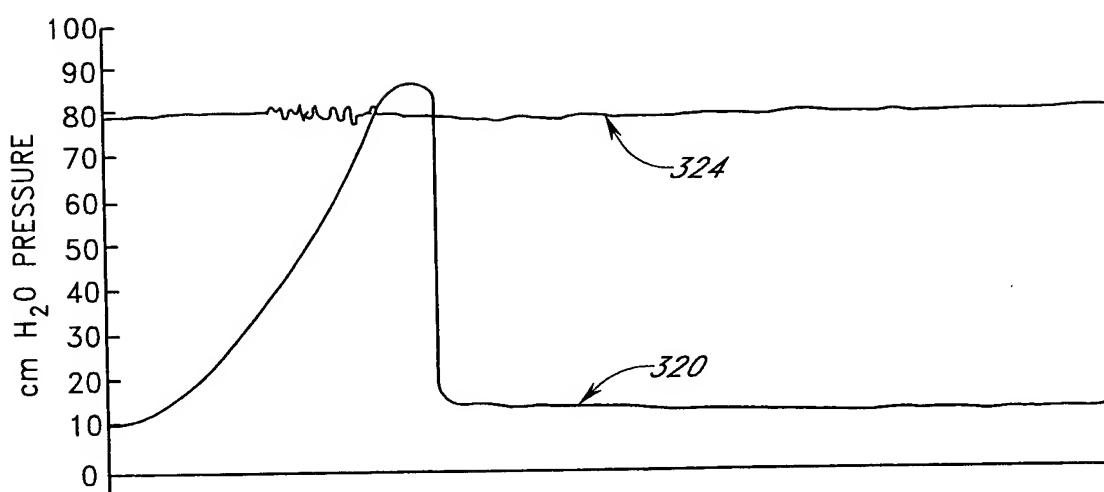


FIG. 2

3/47

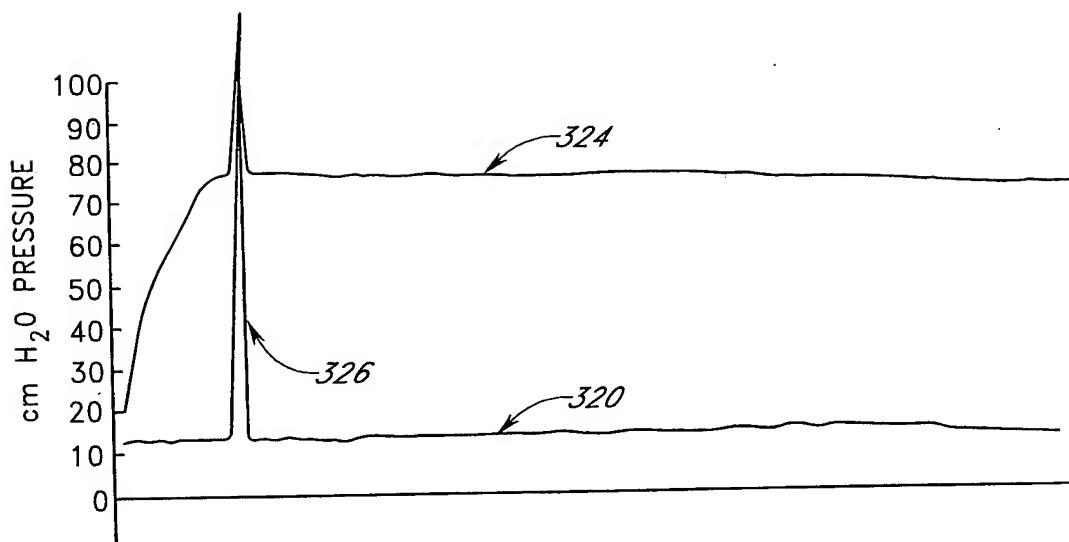


FIG. 3

4/47

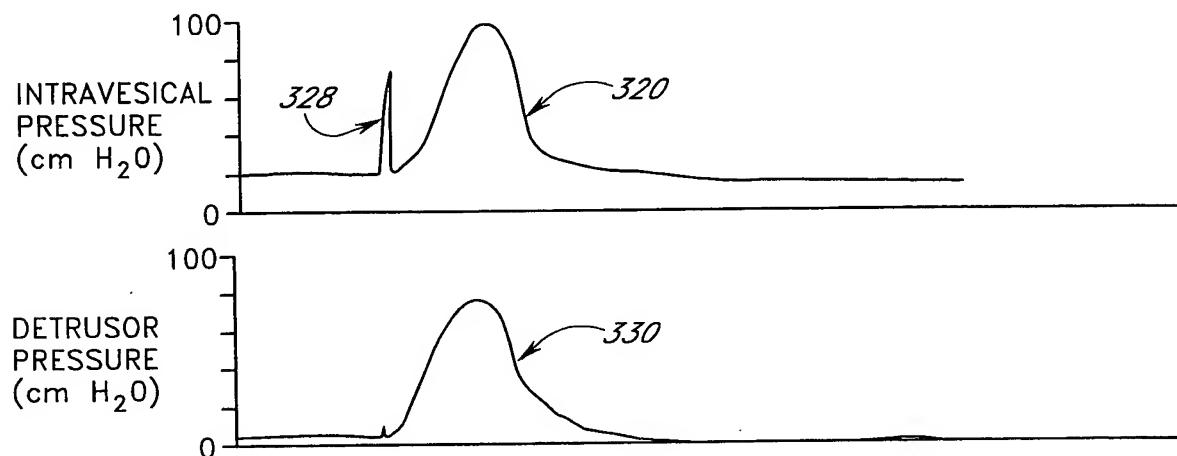


FIG. 4A

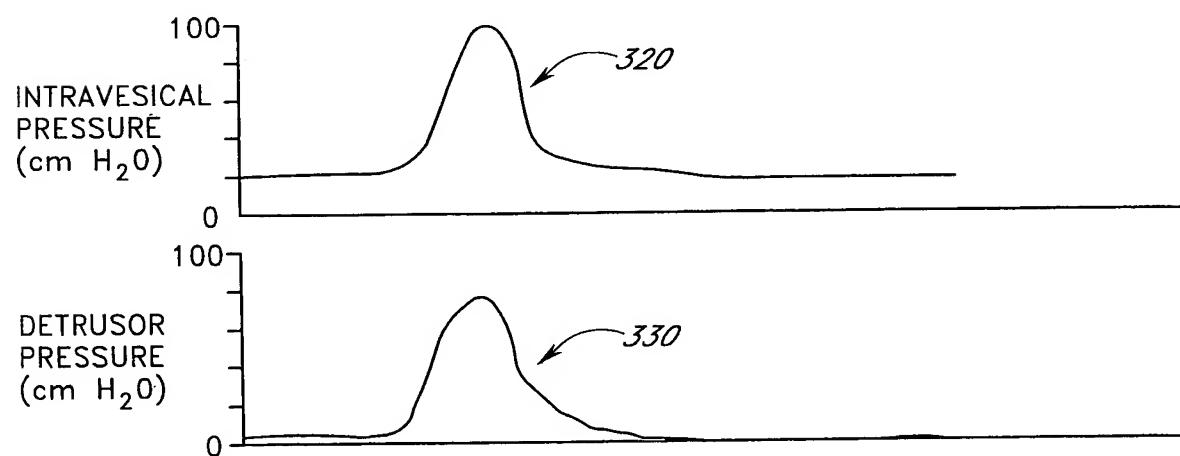


FIG. 4B

HIGH VAPOR PRESSURE ATTENUATION DEVICE
Kevin G. Connors et al.
Appl. No.: Unknown Atty Docket: SOLACE.4CP1C4

5/47

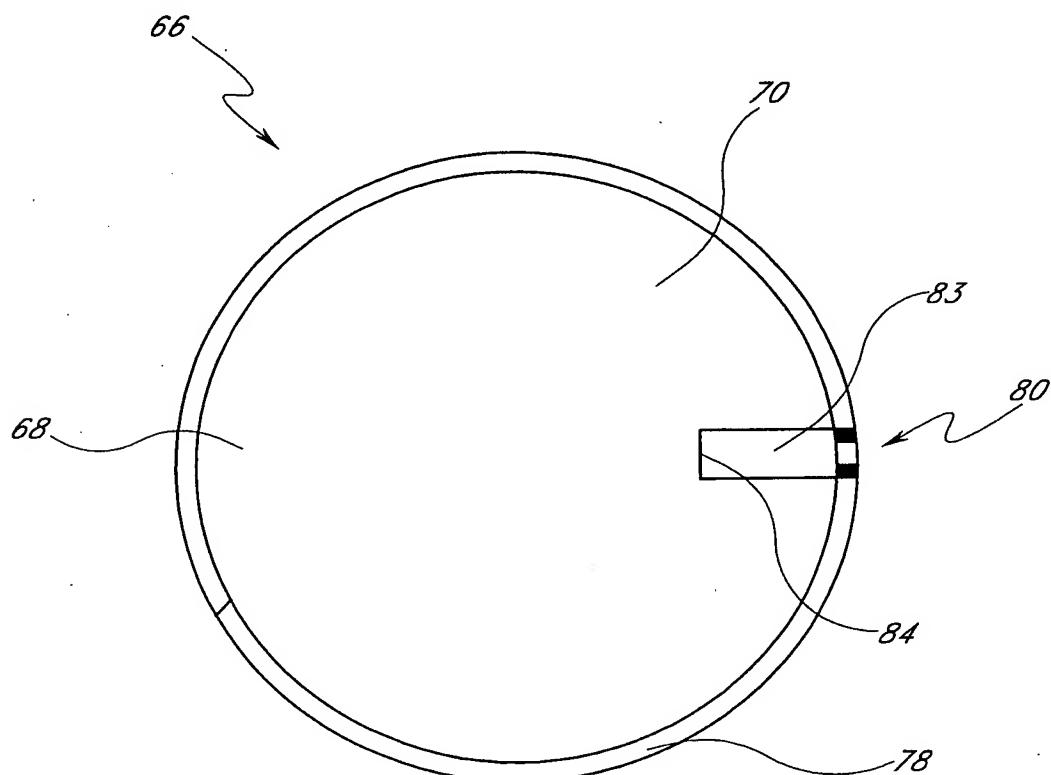


FIG. 5

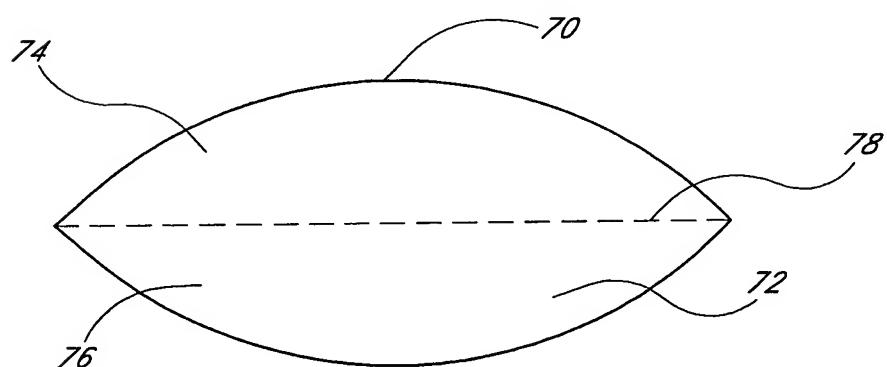


FIG. 5A

HIGH VAPOR PRESSURE ATTENUATION DEVICE

Kevin G. Connors et al.

Appl. No.: Unknown

Atty Docket: SOLACE.4CP1C4

6/47

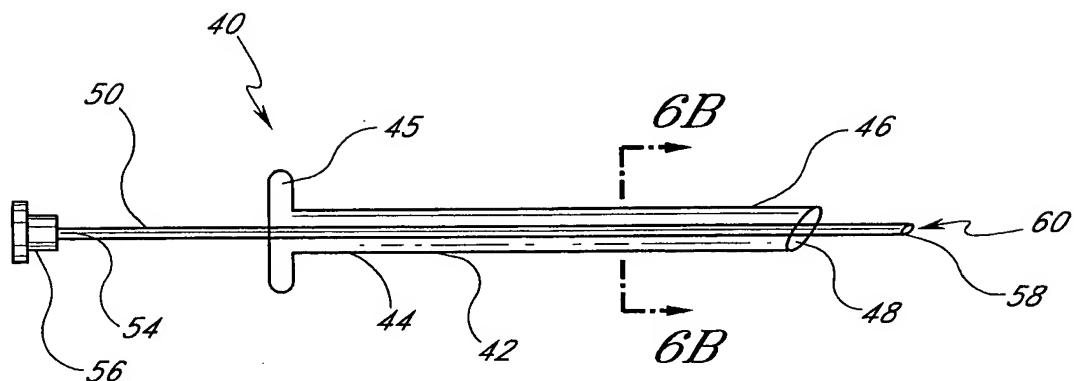


FIG. 6

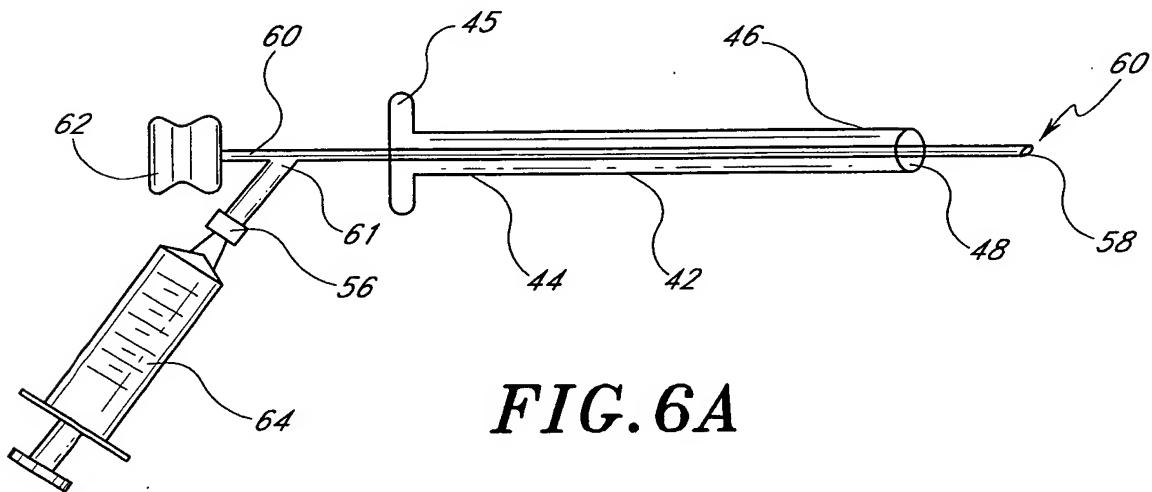


FIG. 6A

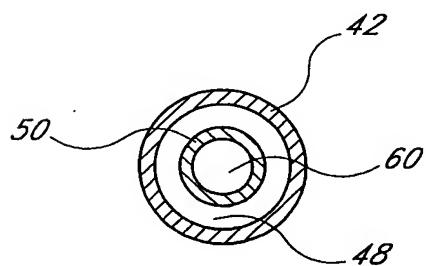


FIG. 6B

HIGH VAPOR PRESSURE ATTENUATION DEVICE
Kevin G. Connors et al.
Appl. No.: Unknown Atty Docket: SOLACE.4CPIC4

7/47

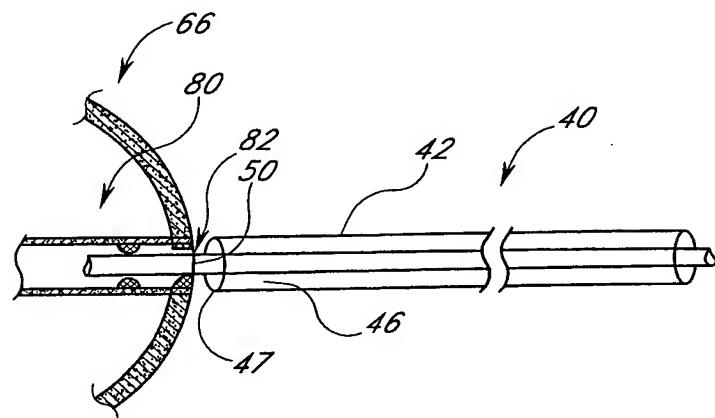


FIG. 7A

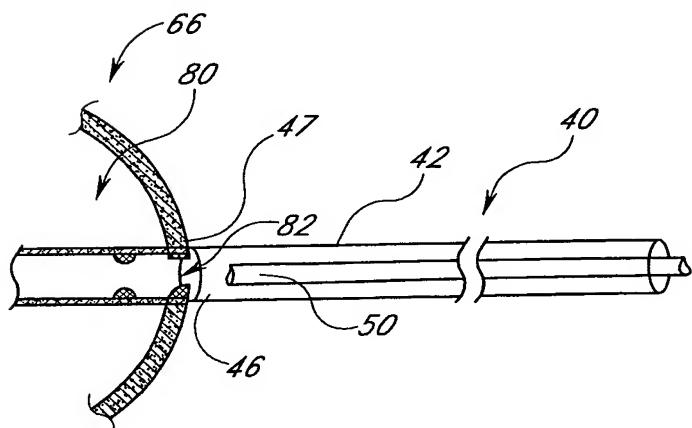


FIG. 7B

8/47

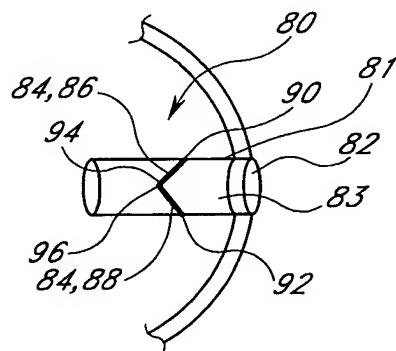


FIG. 8A

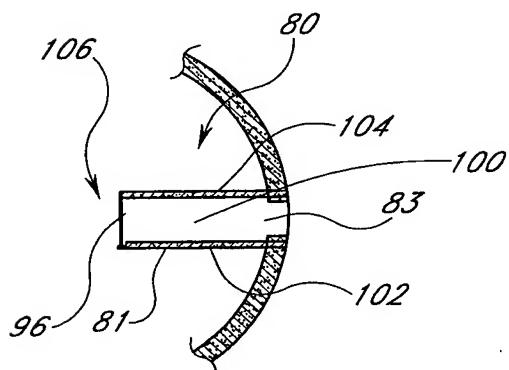


FIG. 8B

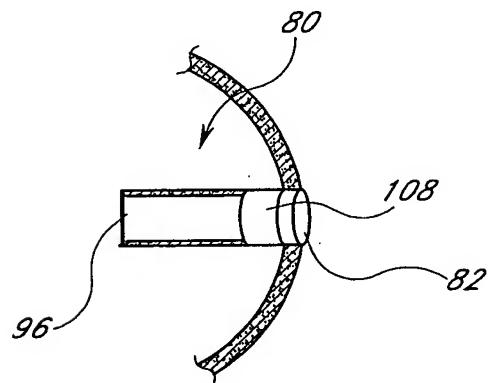


FIG. 8C

9 / 47

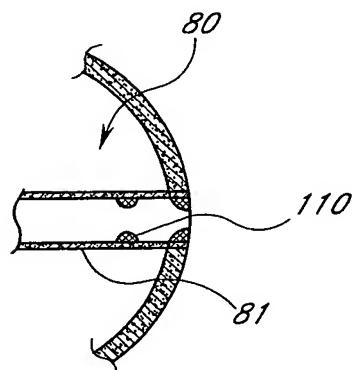


FIG. 8D

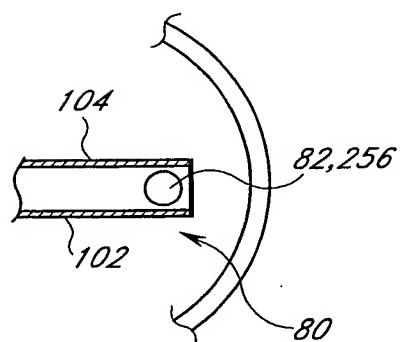


FIG. 8E

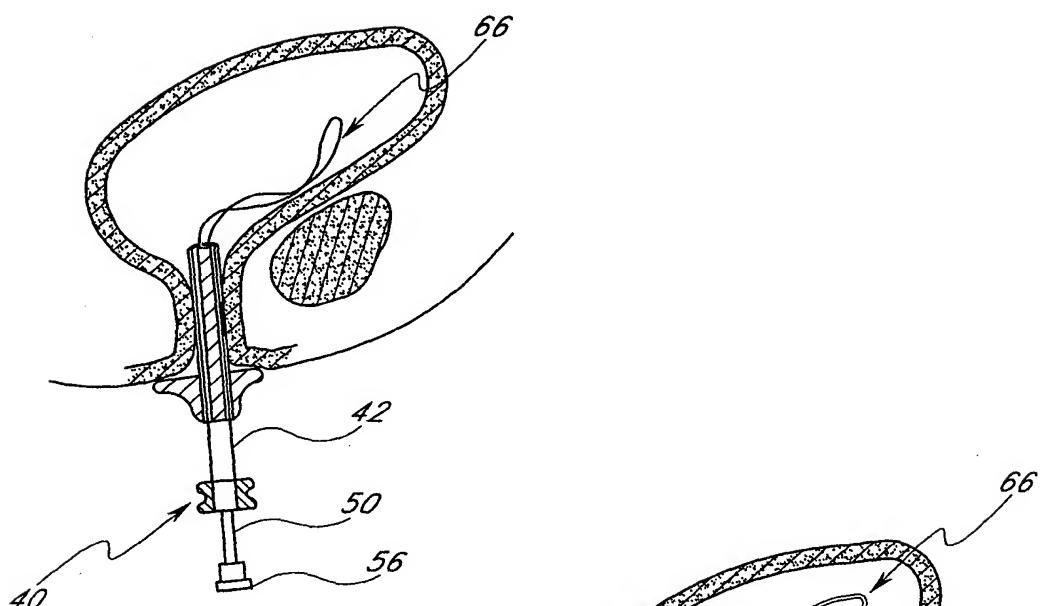


FIG. 9

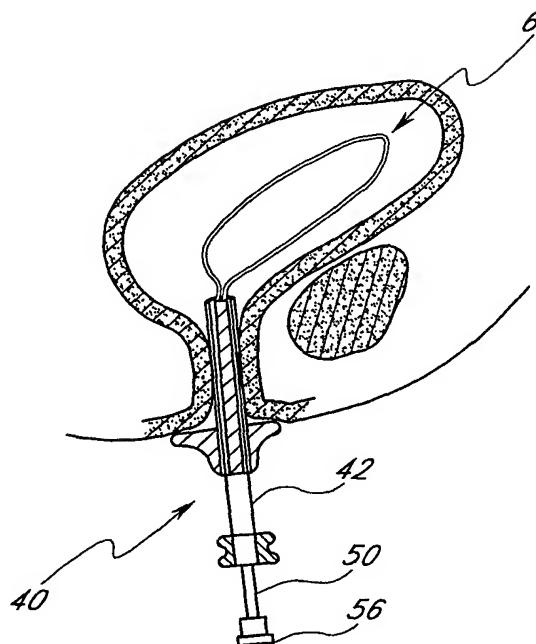


FIG. 10

HIGH VAPOR PRESSURE ATTENUATION DEVICE

Kevin G. Connors et al.

Appl. No.: Unknown Atty Docket: SOLACE.4CP1C4

11/47

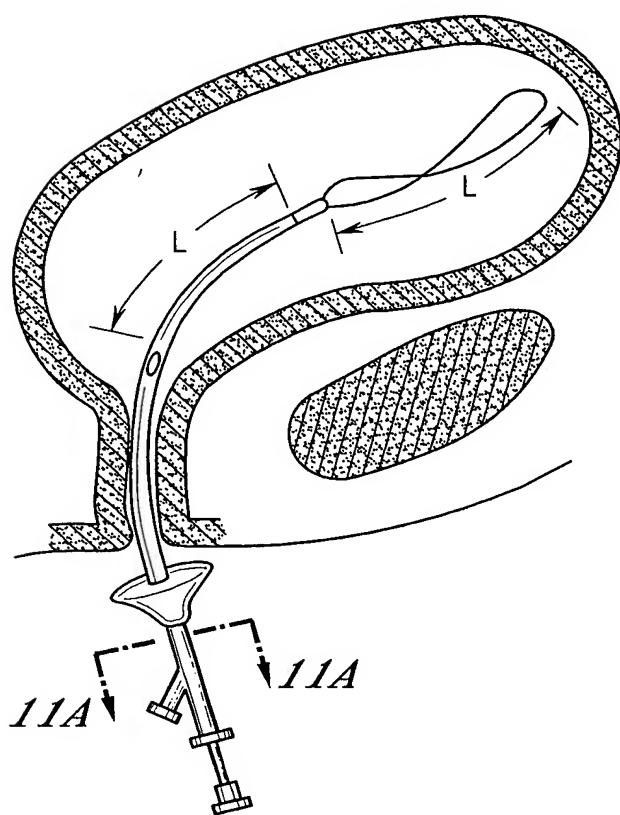


FIG. 11




FIG. 11A

HIGH VAPOR PRESSURE ATTENUATION DEVICE

Kevin G. Connors et al.

Appl. No.: Unknown Atty Docket: SOLACE.4CP1C4

12/47

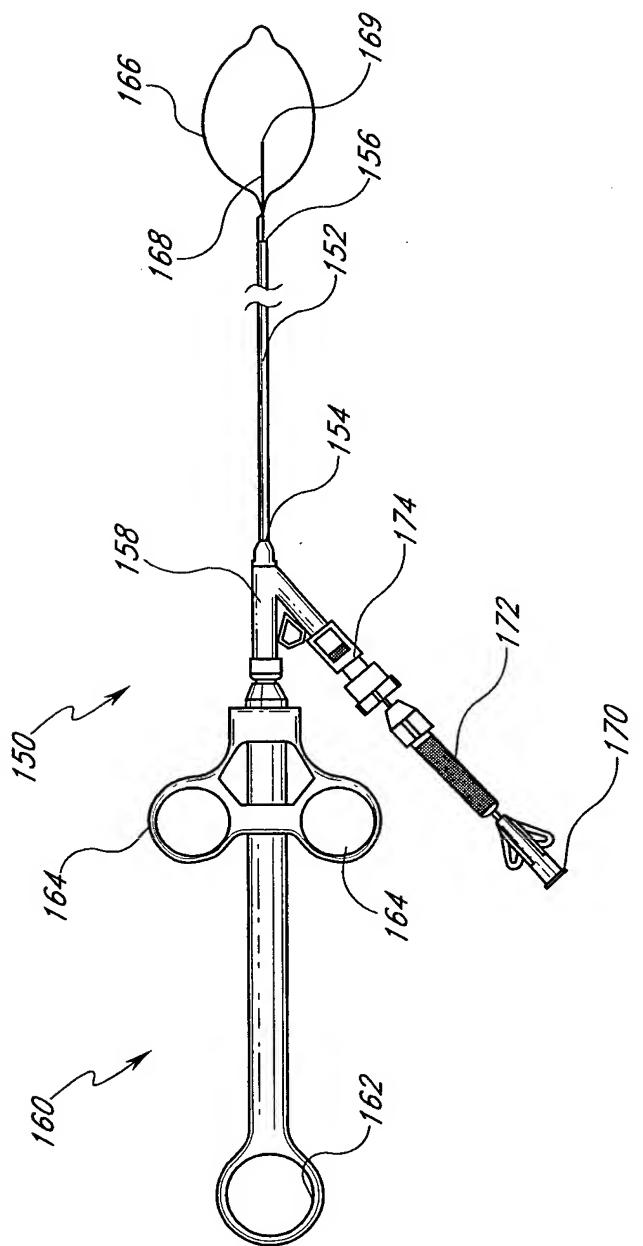


FIG. 12

13/47

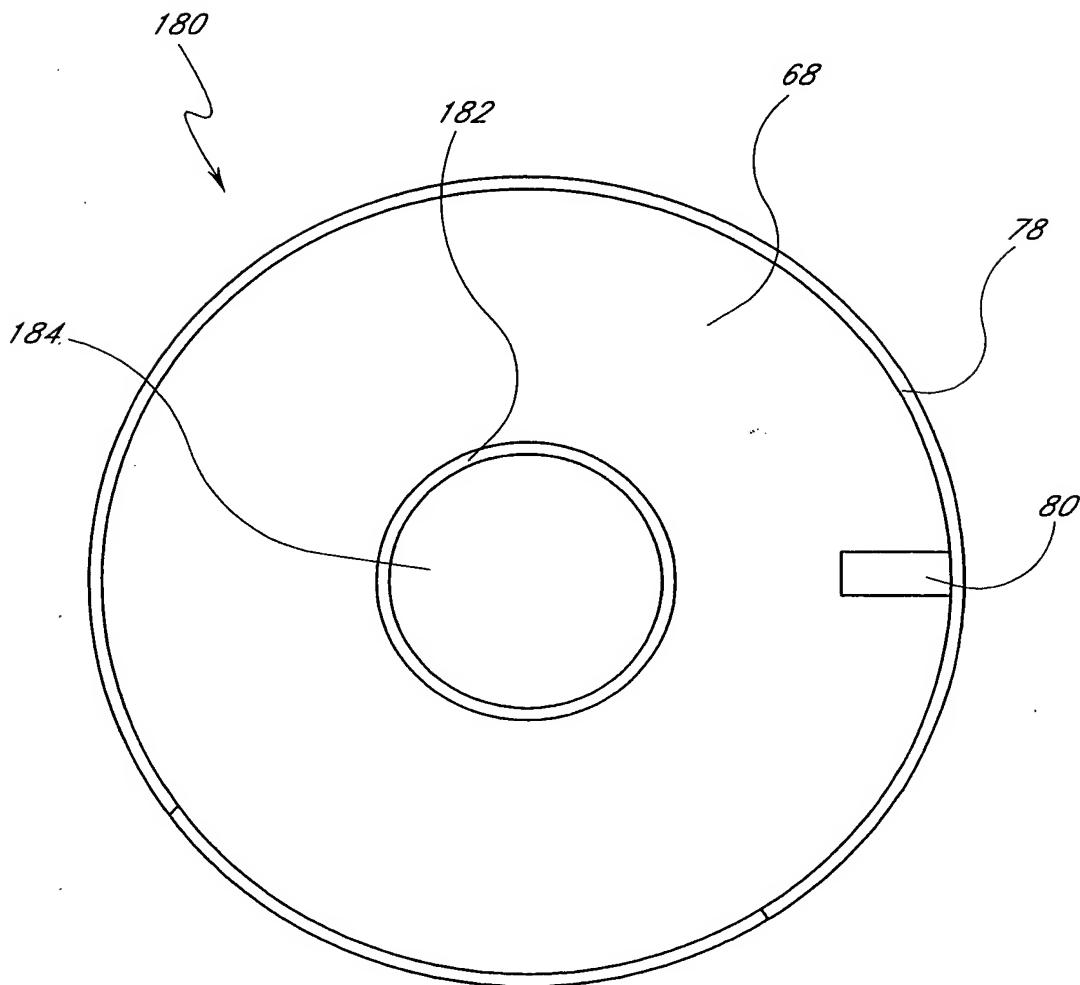


FIG. 13

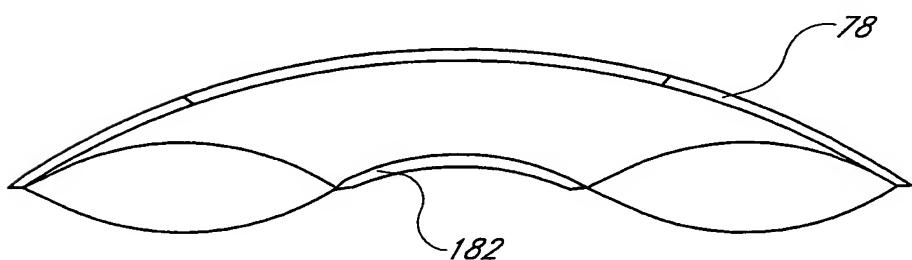


FIG. 13A

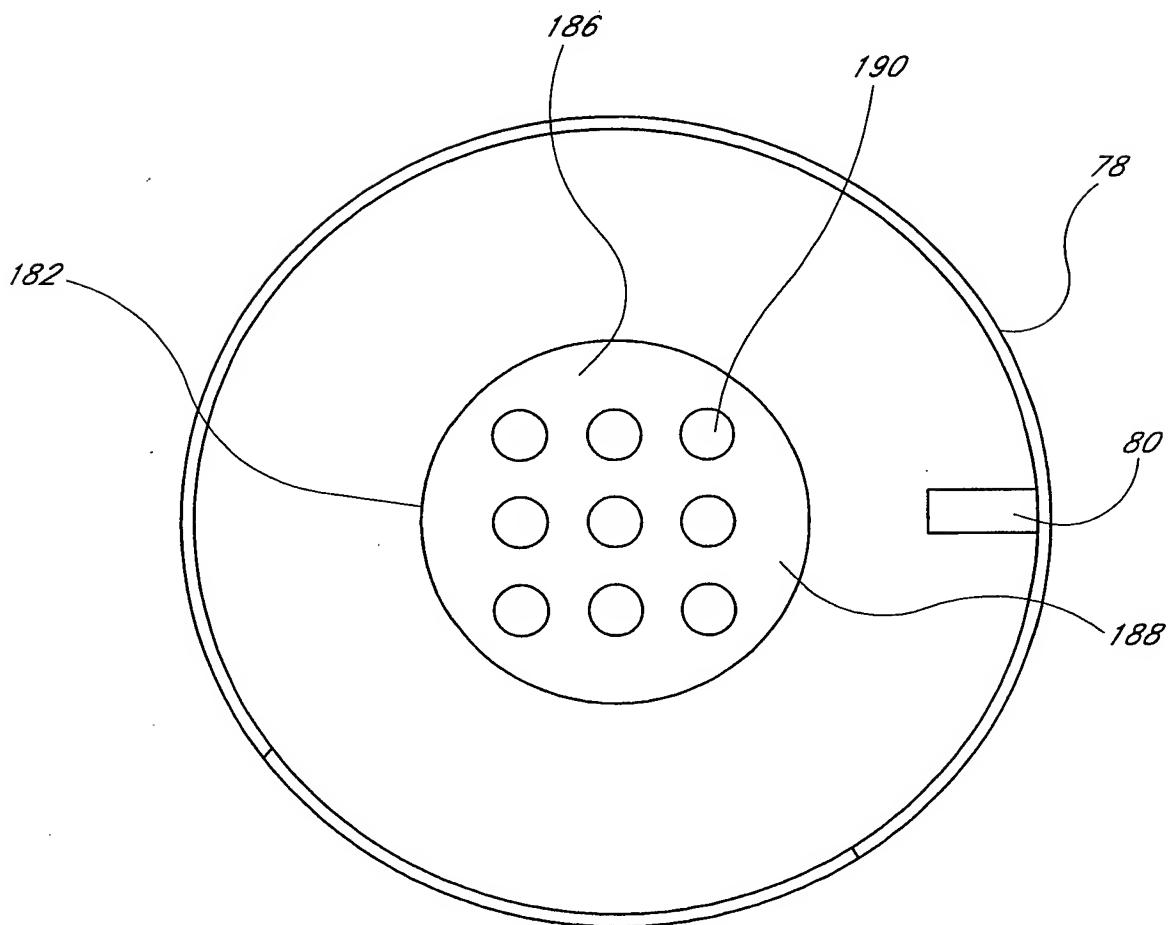


FIG. 14

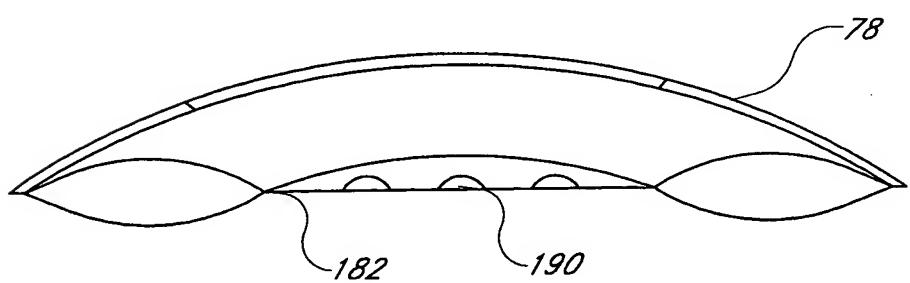


FIG. 14A

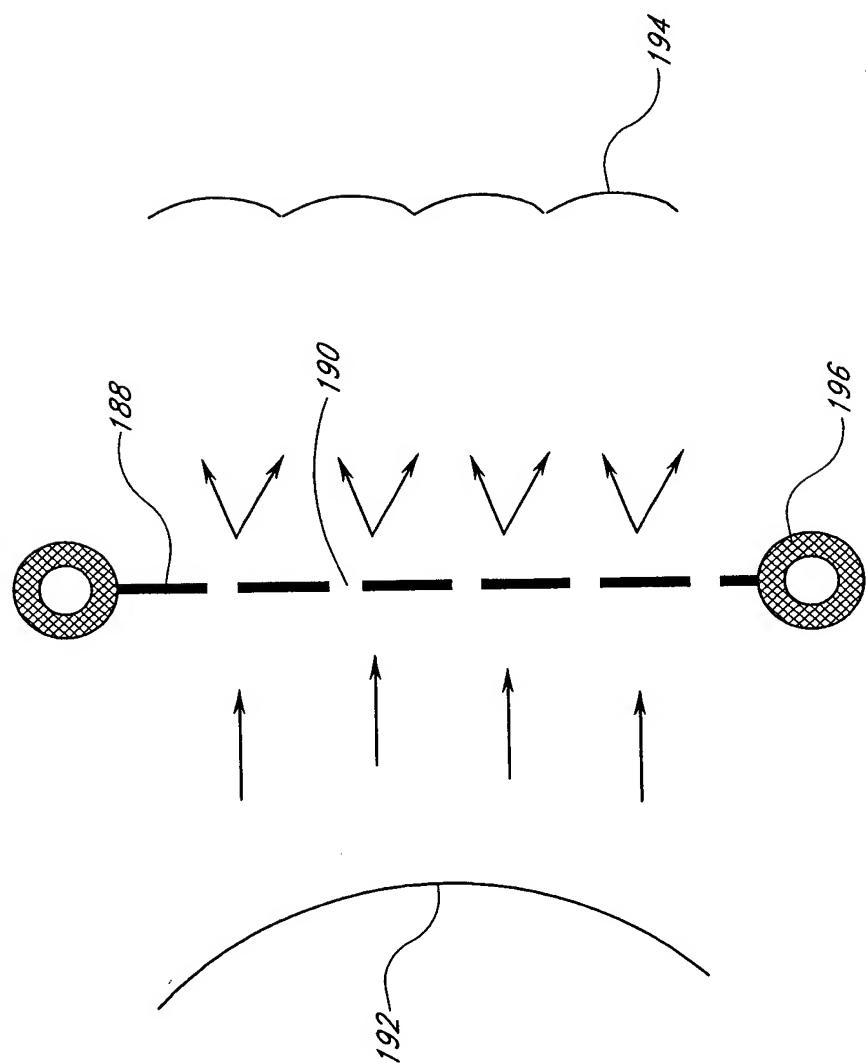


FIG. 15

FIG. 16A

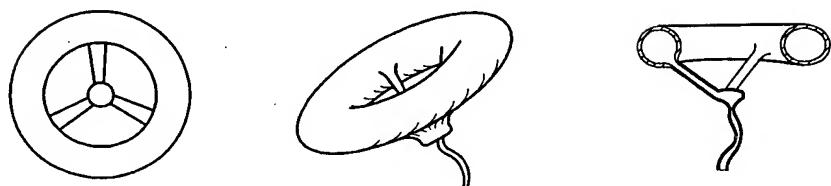


FIG. 16B

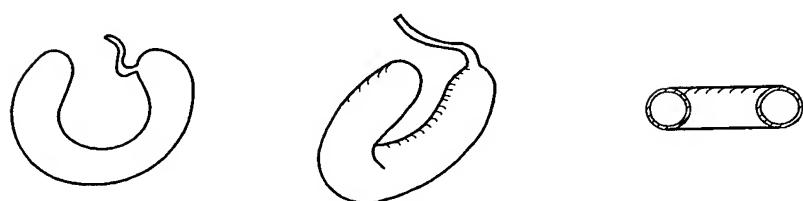


FIG. 16C



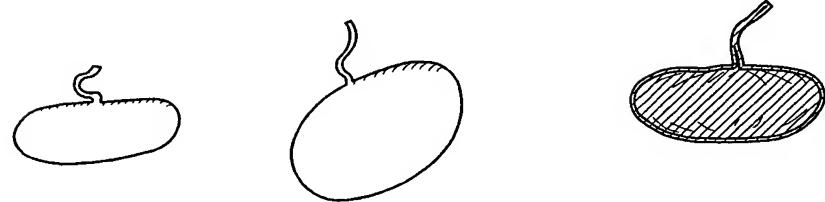


FIG. 16D

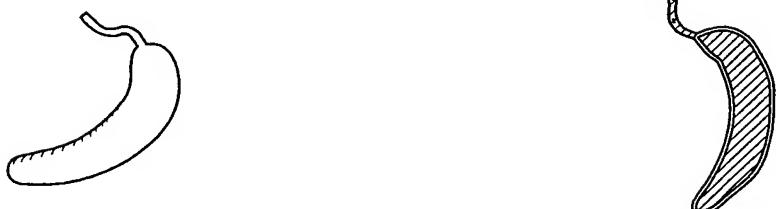

HIGH VAPOR PRESSURE ATTENUATION DEVICE
Kevin G. Connors et al.
Appl. No.: Unknown Atty Docket: SOLACE.4CP1C4

17/47

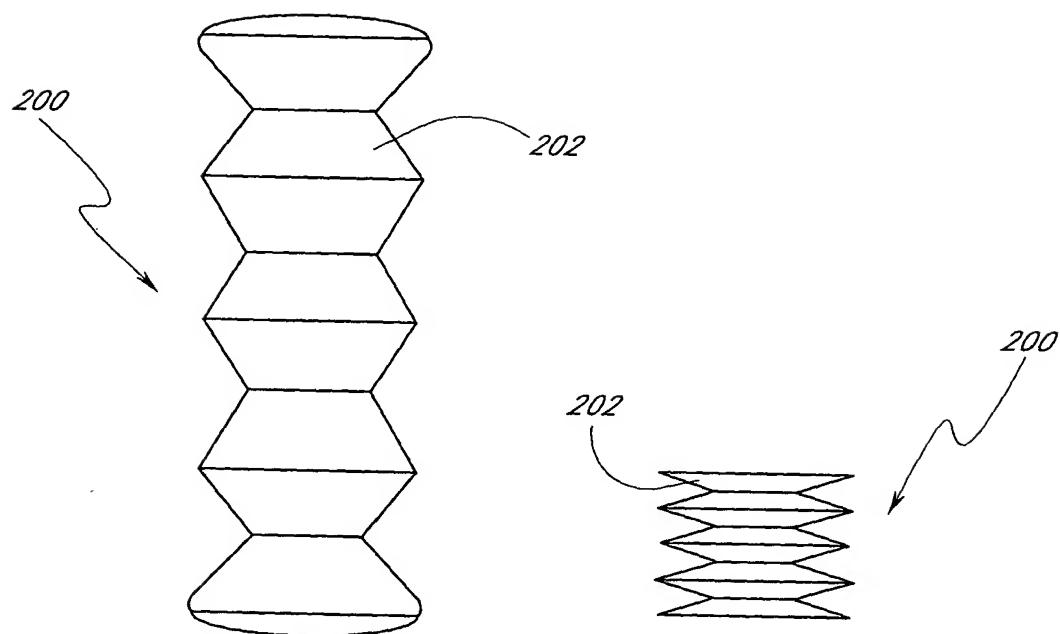

HIGH VAPOR PRESSURE ATTENUATION DEVICE

Kevin G. Connors et al.

Appl. No.: Unknown Atty Docket: SOLACE.4CP1C4

18/47

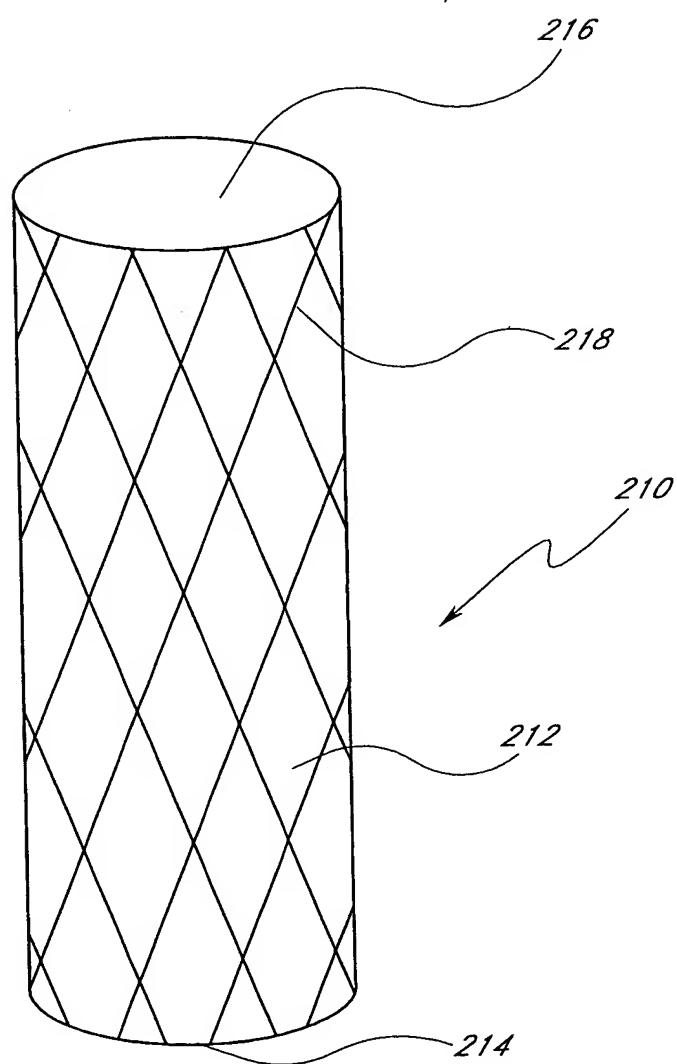


FIG. 18

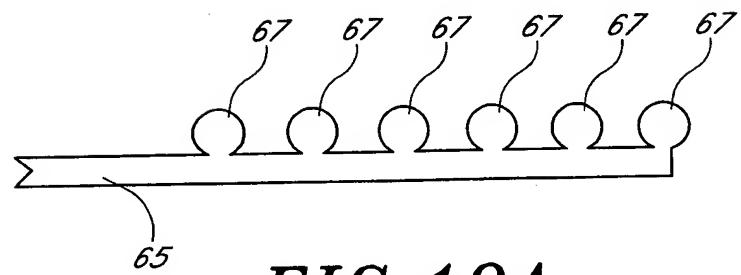


FIG. 19A

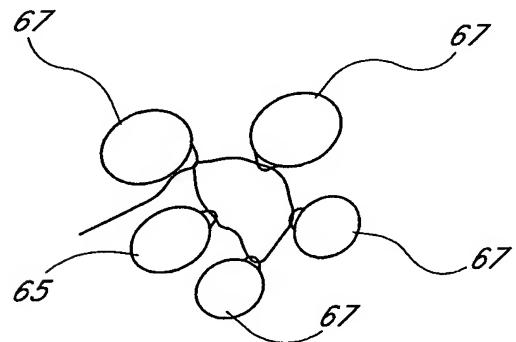


FIG. 19B

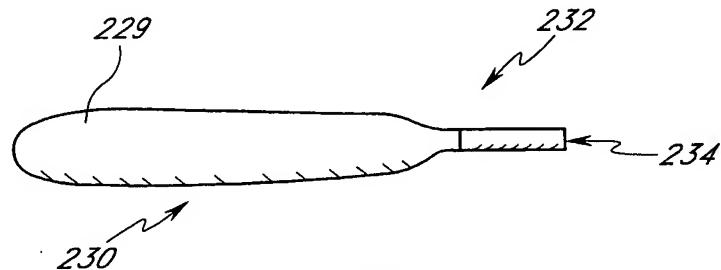


FIG. 20

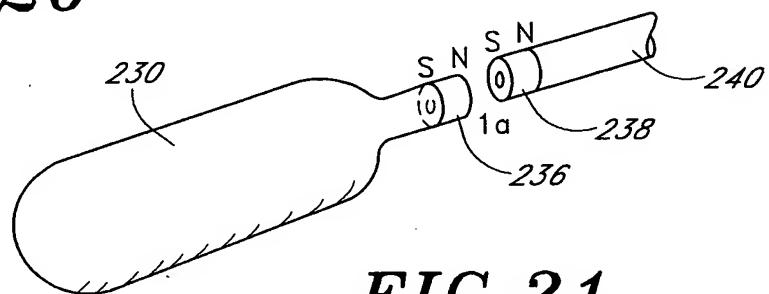


FIG. 21

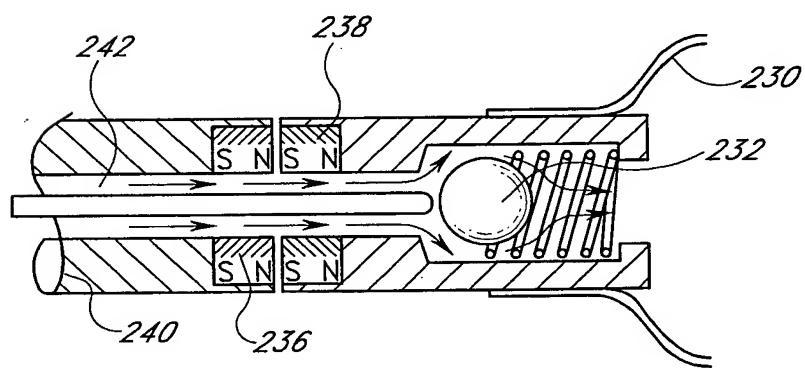


FIG. 22

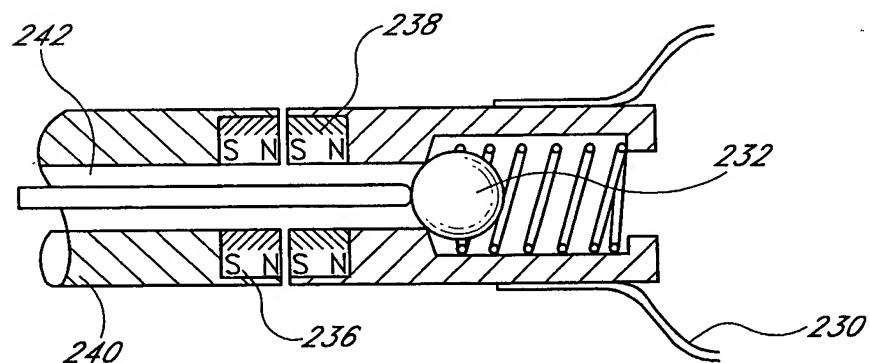


FIG. 23

HIGH VAPOR PRESSURE ATTENUATION DEVICE

Kevin G. Connors et al.

Appl. No.: Unknown Atty Docket: SOLACE.4CP1C4

21/47

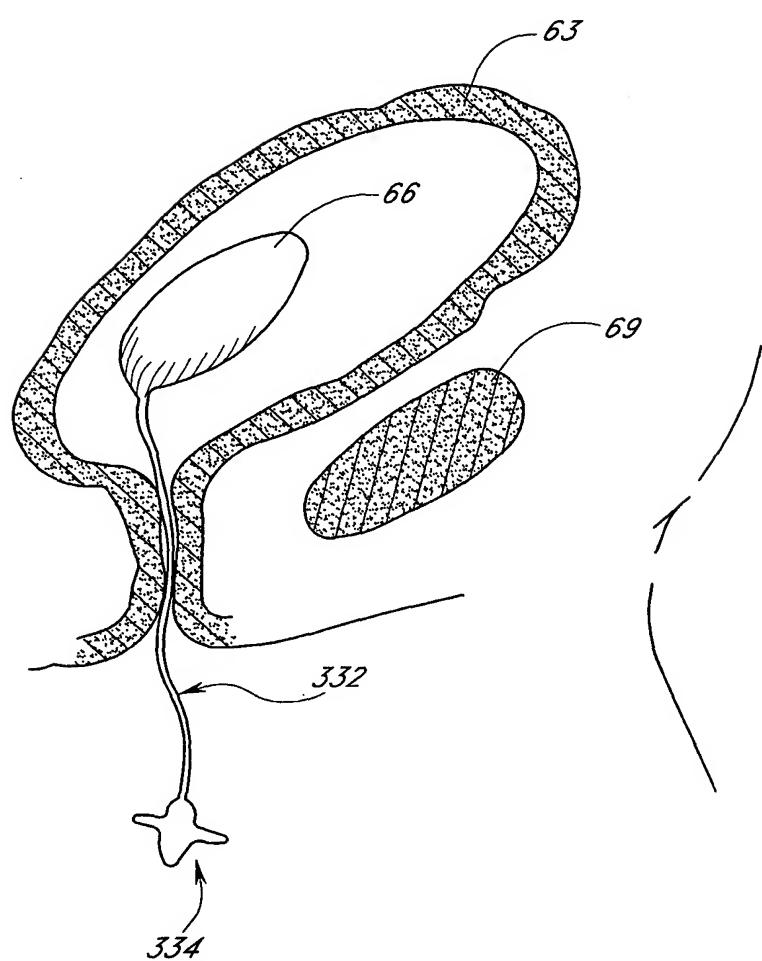


FIG. 24

HIGH VAPOR PRESSURE ATTENUATION DEVICE

Kevin G. Connors et al.

Appl. No.: Unknown Atty Docket: SOLACE.4CP1C4

22/47

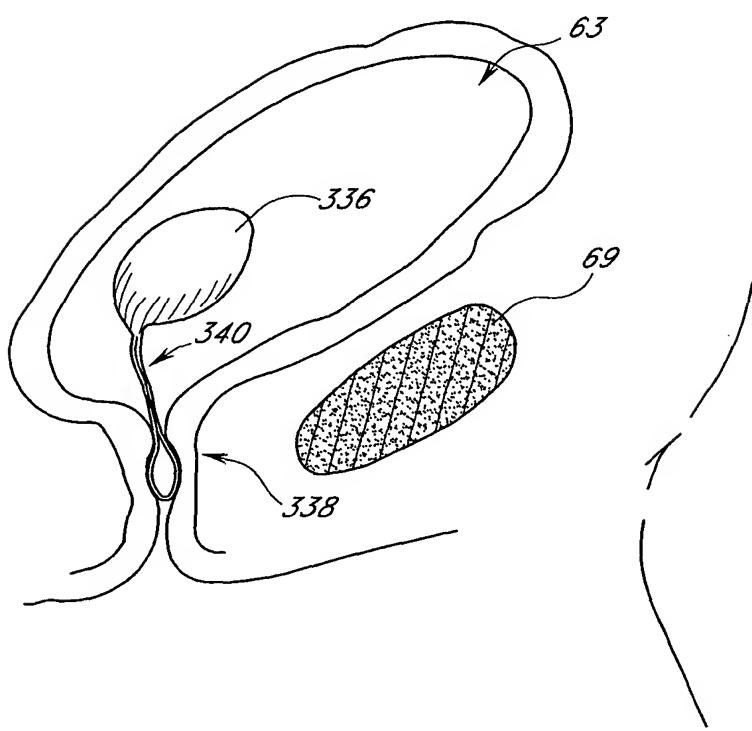


FIG.25

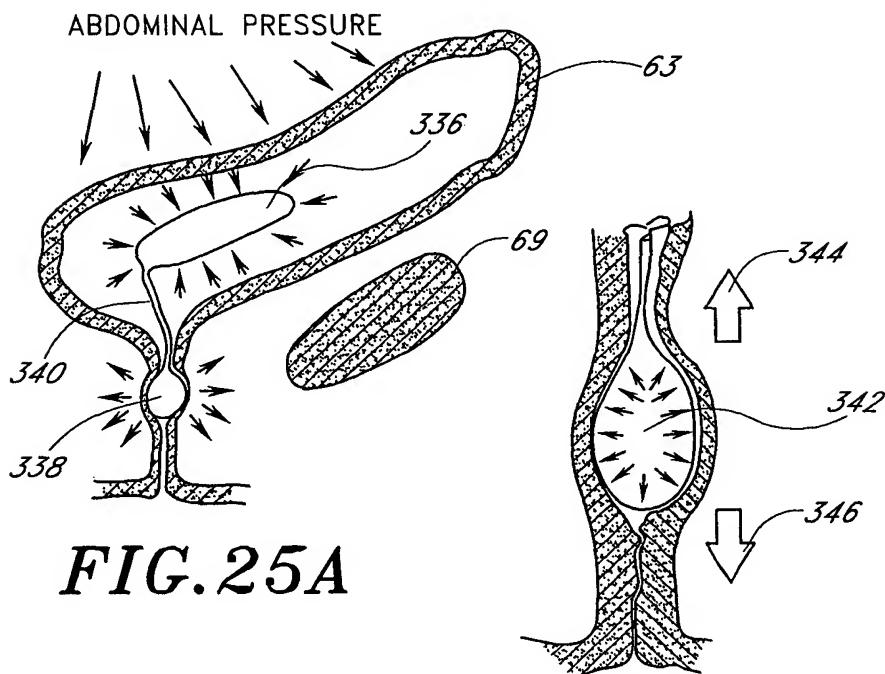


FIG. 25A

FIG. 25B

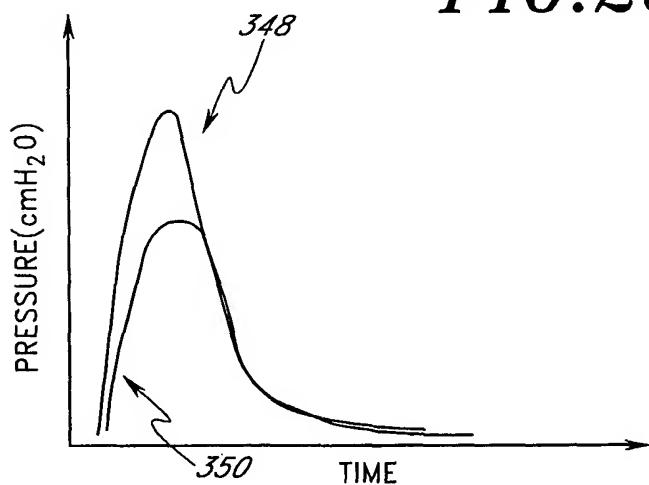


FIG. 25C

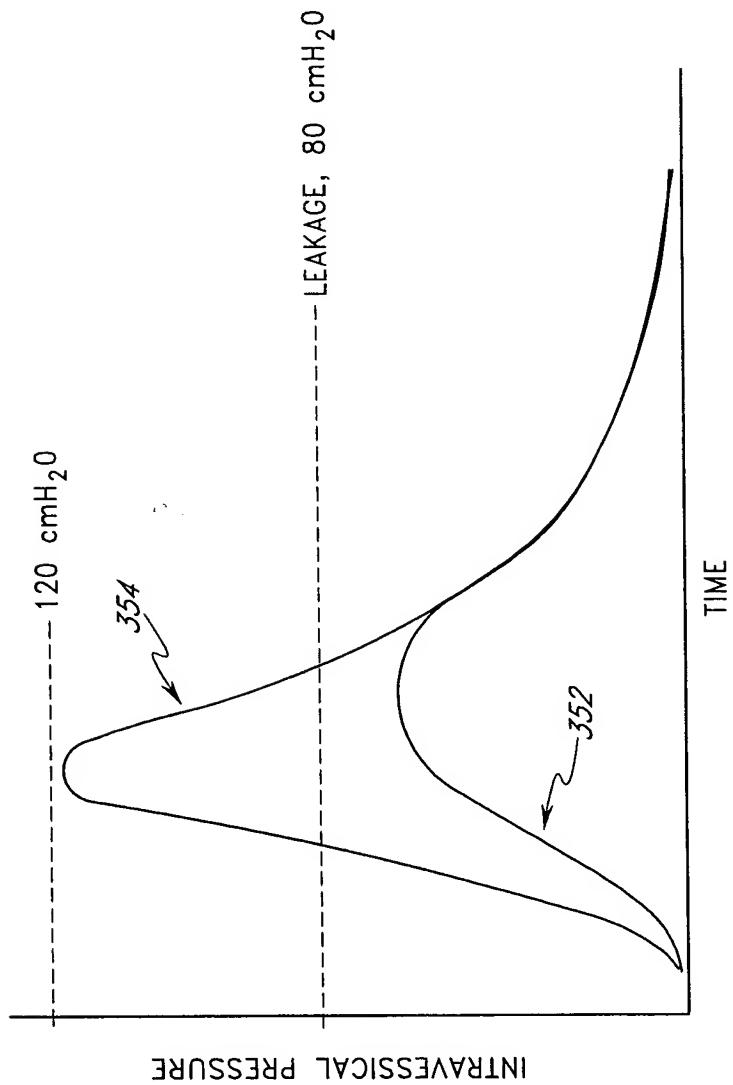


FIG. 26

HIGH VAPOR PRESSURE ATTENUATION DEVICE

Kevin G. Connors et al.

Appl. No.: Unknown Atty Docket: SOLACE.4CP1C4

25/47

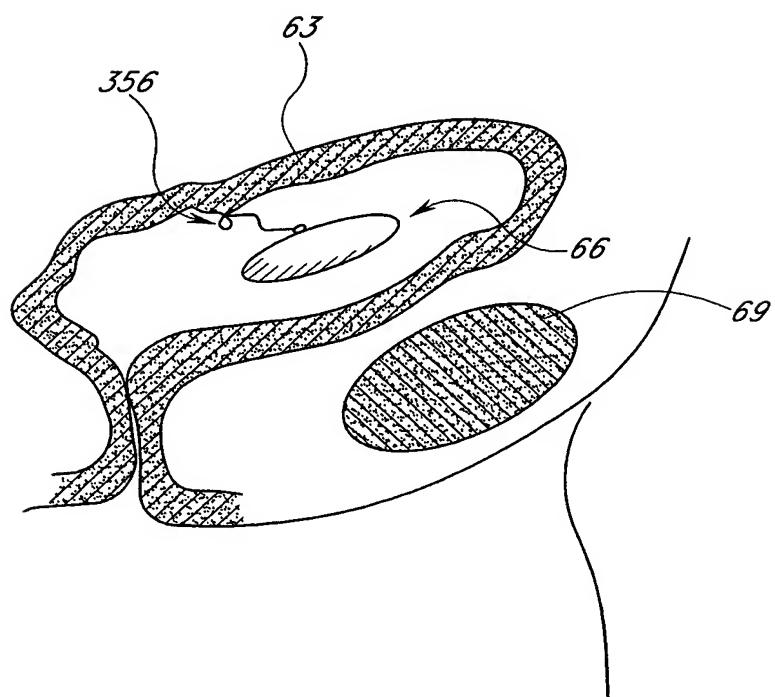


FIG. 27

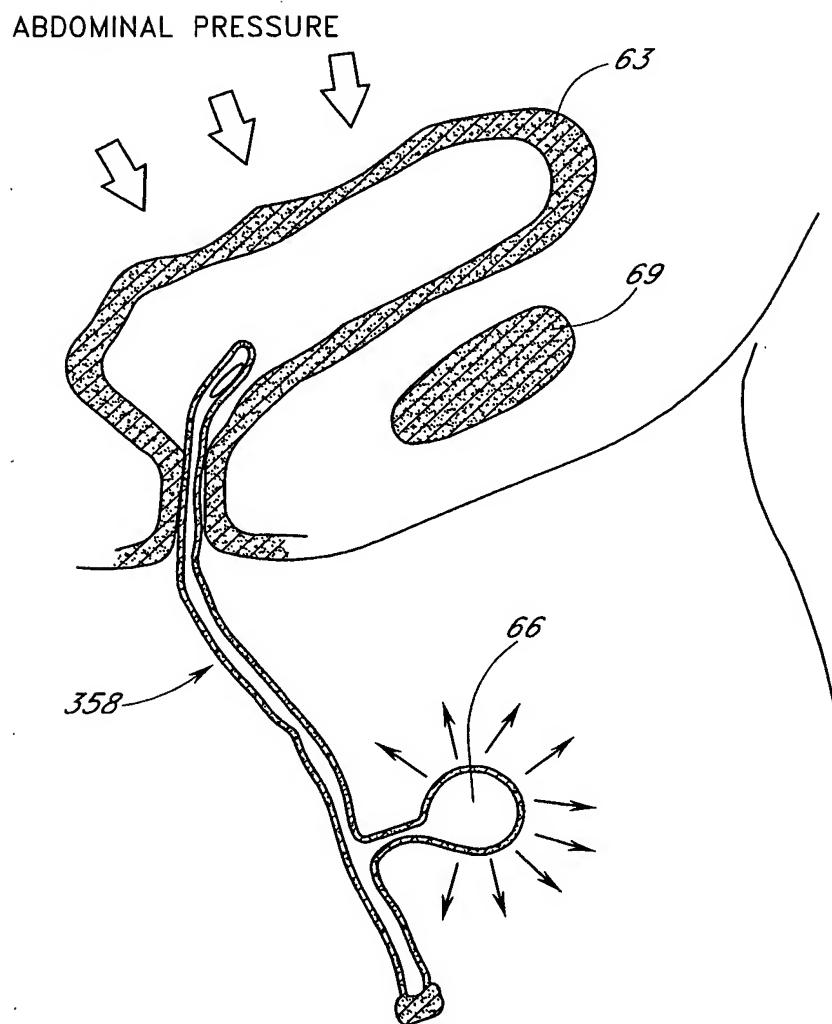


FIG. 28

HIGH VAPOR PRESSURE ATTENUATION DEVICE

Kevin G. Connors et al.

Appl. No.: Unknown Atty Docket: SOLACE.4CP1C4

27/47

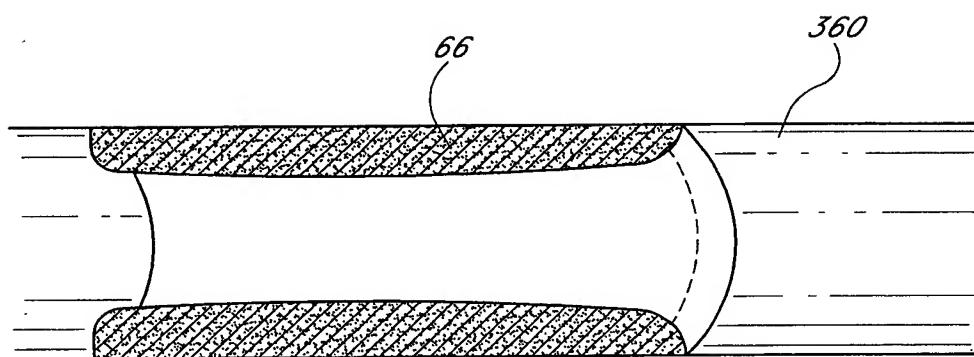


FIG. 29

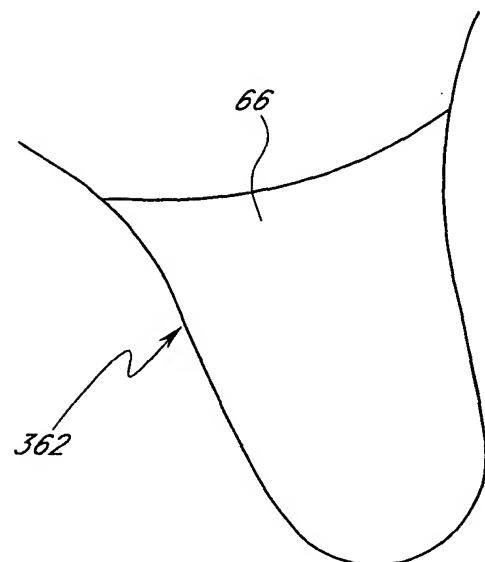


FIG. 30A

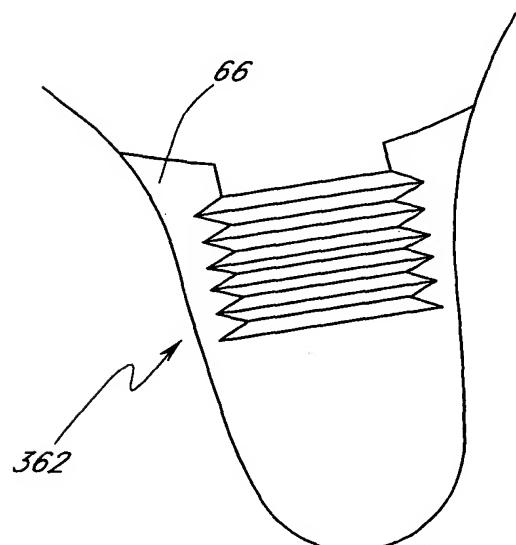


FIG. 30B

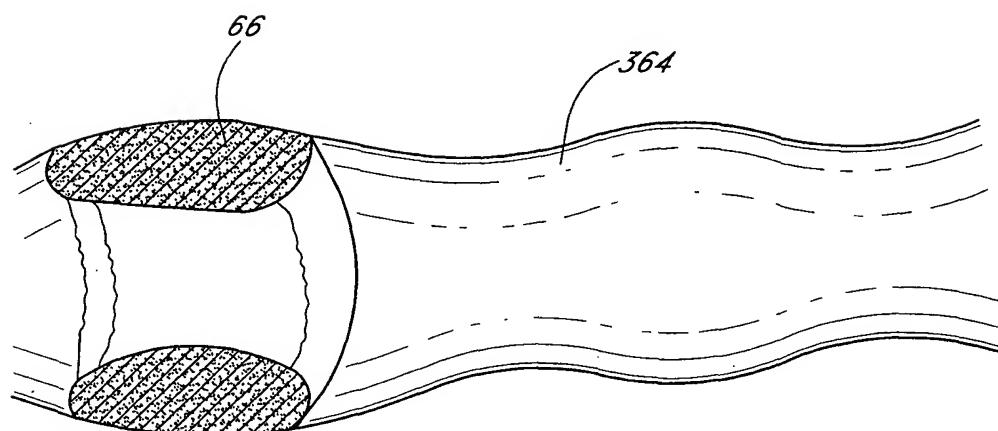


FIG. 31

HIGH VAPOR PRESSURE ATTENUATION DEVICE

Kevin G. Connors et al.

Appl. No.: Unknown Atty Docket: SOLACE.4CP1C4

30/47

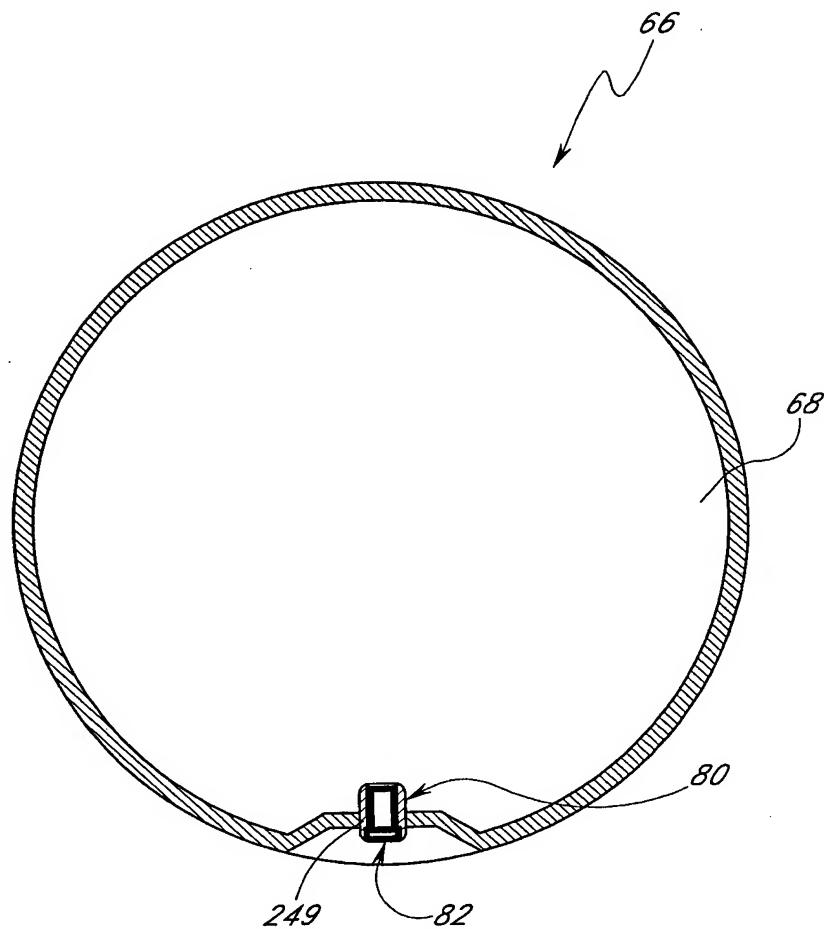


FIG. 32A

HIGH VAPOR PRESSURE ATTENUATION DEVICE

Kevin G. Connors et al.

Appl. No.: Unknown Atty Docket: SOLACE.4CP1C4

31 / 4.7

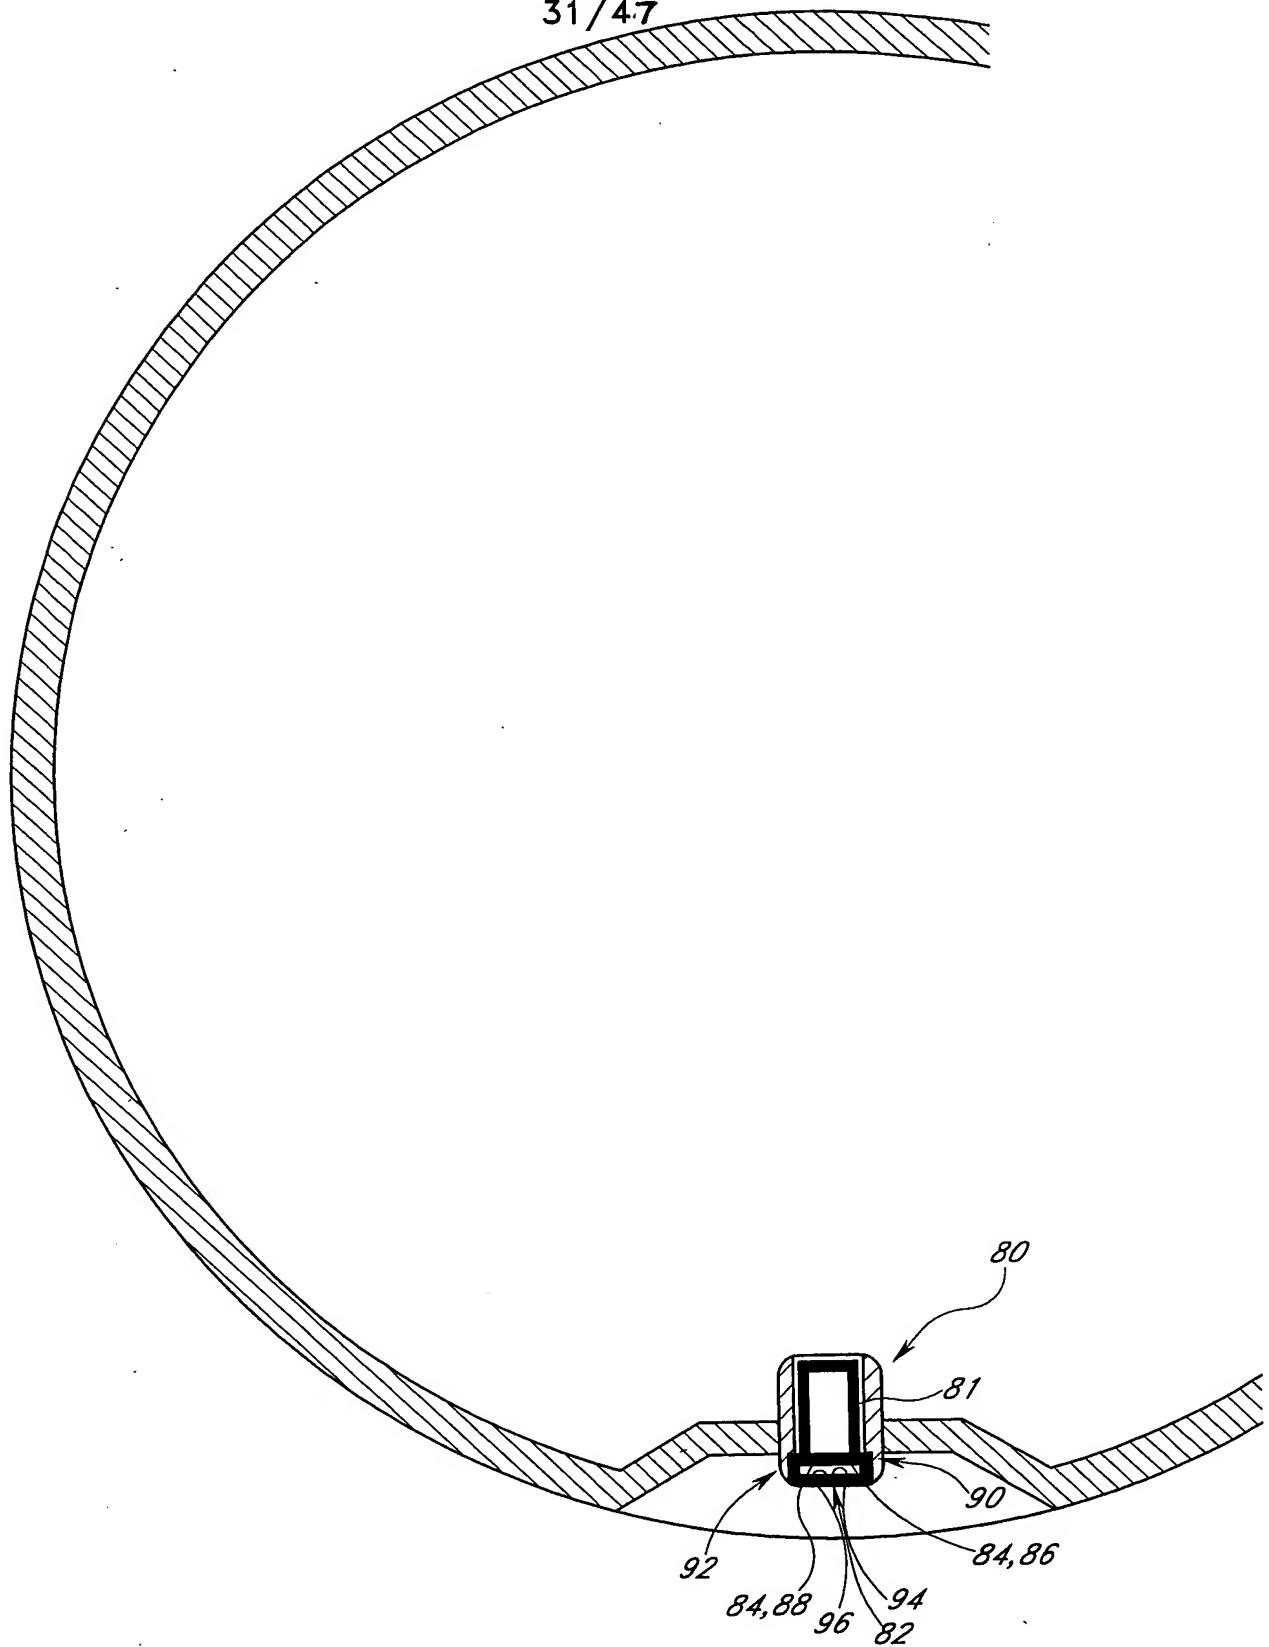


FIG. 32B

HIGH VAPOR PRESSURE ATTENUATION DEVICE
Kevin G. Connors et al.
Appl. No.: Unknown Atty Docket: SOLACE.4CP1C4

32/47

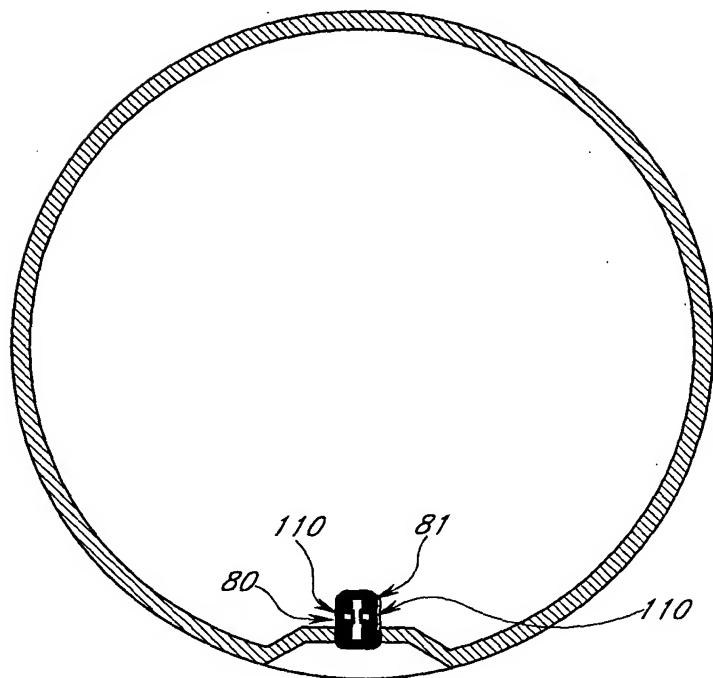


FIG. 33A

33/47

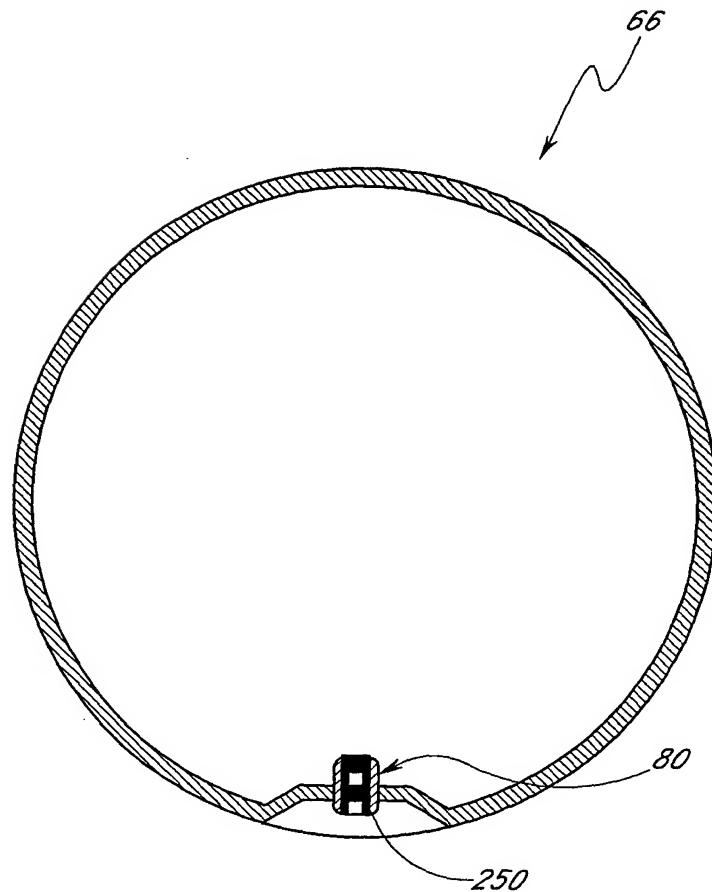


FIG. 33B

34/47

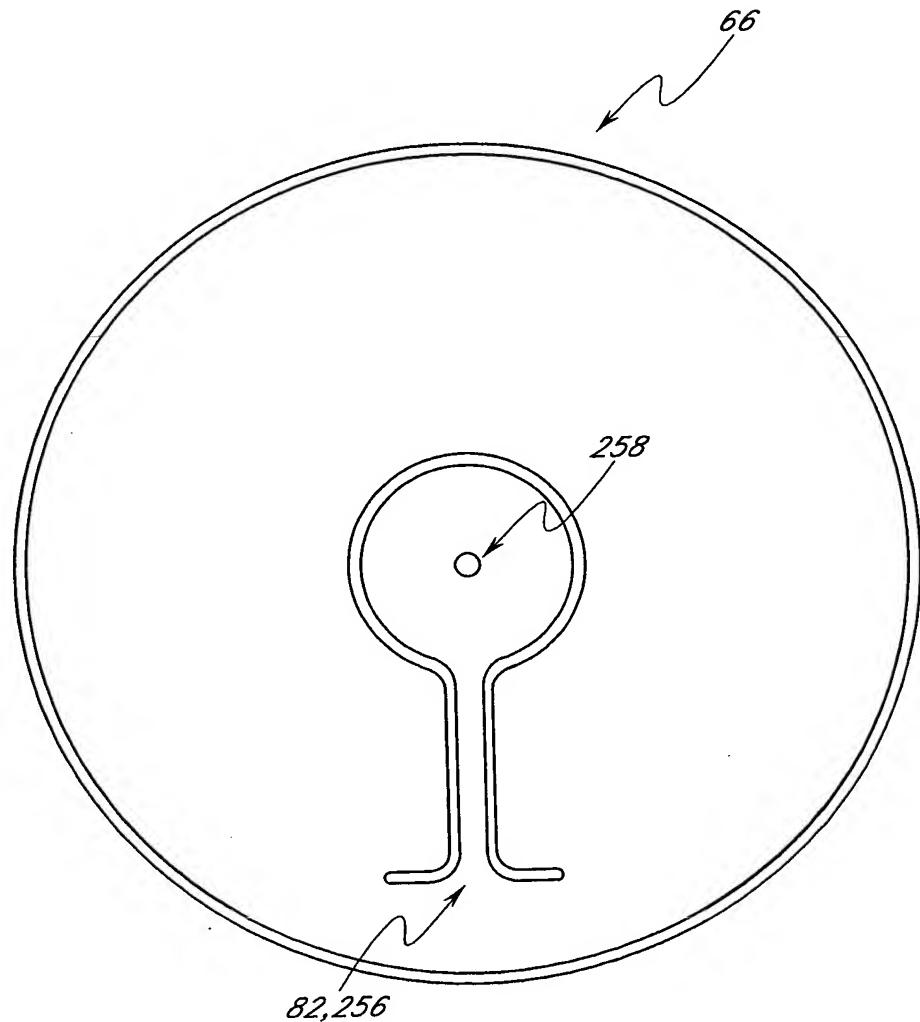


FIG. 33C

HIGH VAPOR PRESSURE ATTENUATION DEVICE
Kevin G. Connors et al.
Appl. No.: Unknown Atty Docket: SOLACE.4CPI.C4

35/47

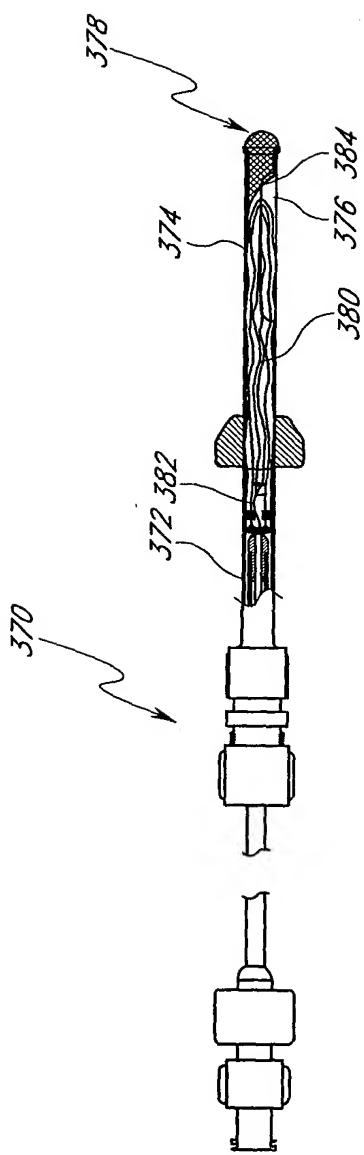


FIG. 34A

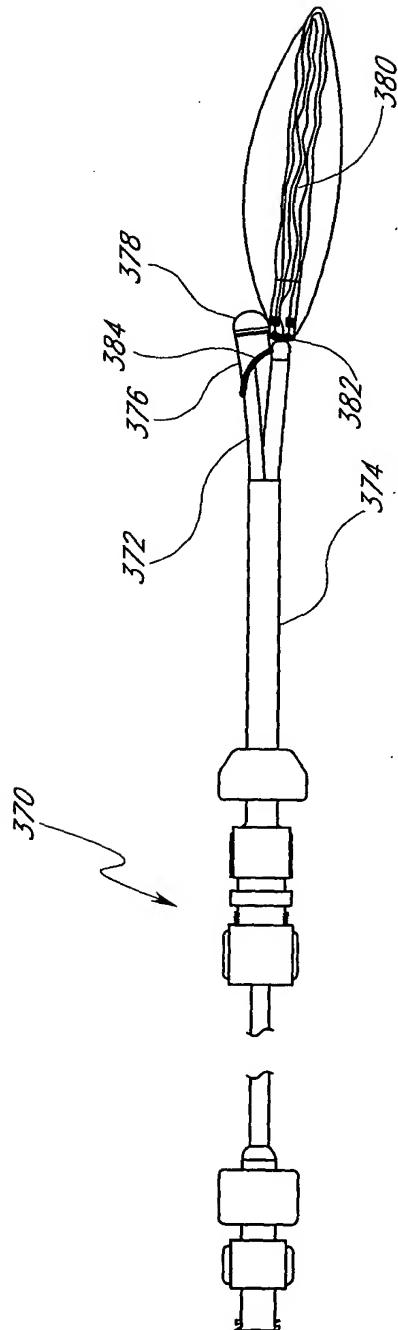


FIG. 34B

HIGH VAPOR PRESSURE ATTENUATION DEVICE

Kevin G. Connors et al.

Appl. No.: Unknown Atty Docket: SOLACE.4CP1C4

36/47

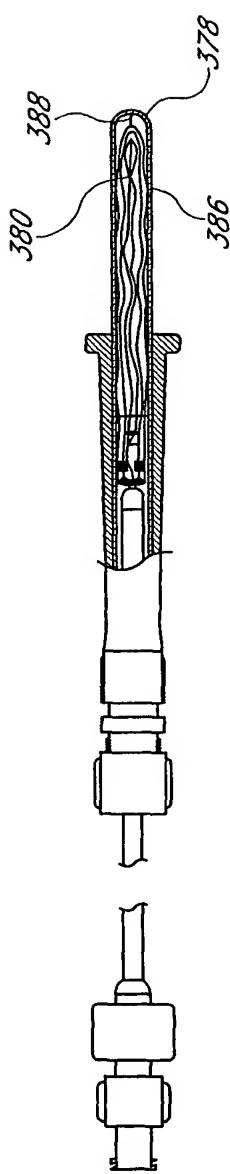


FIG. 35A

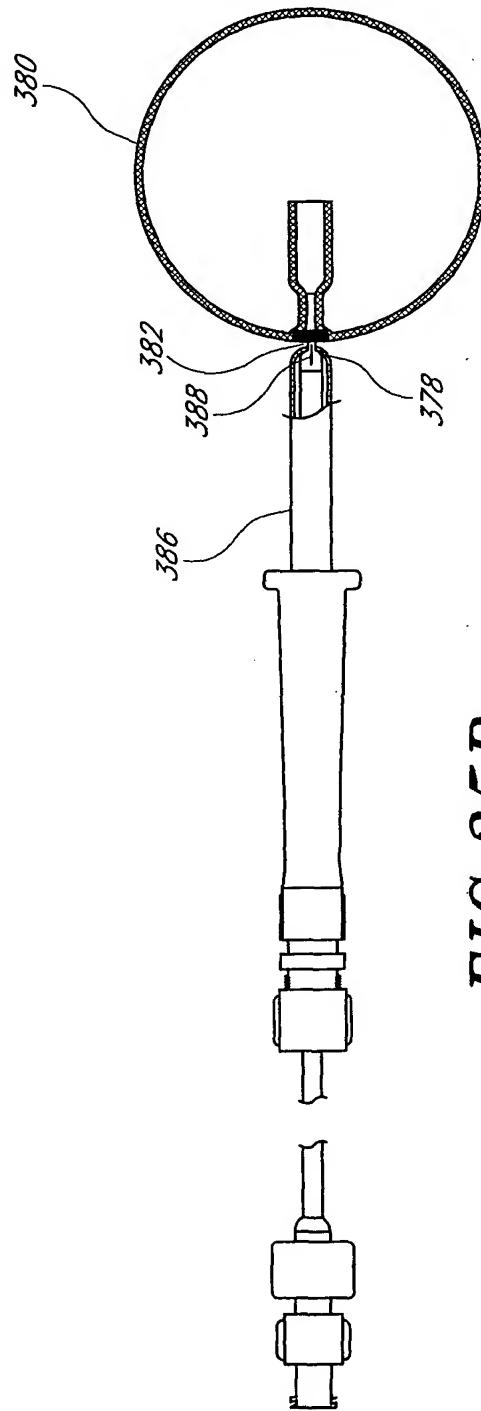


FIG. 35B

HIGH VAPOR PRESSURE ATTENUATION DEVICE
Kevin G. Connors et al.
Appl. No.: Unknown Atty Docket: SOLACE.4CP1C4

37/47

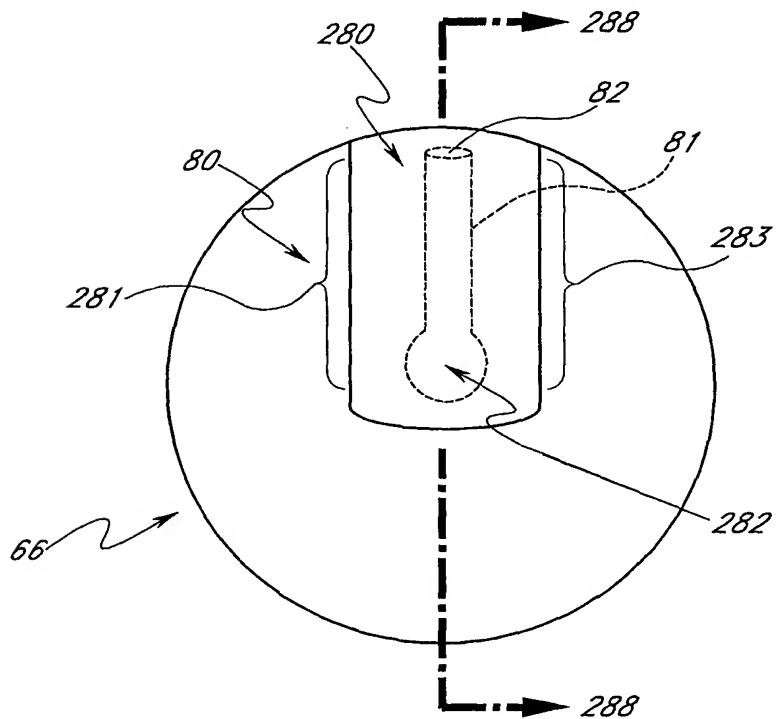


FIG. 36

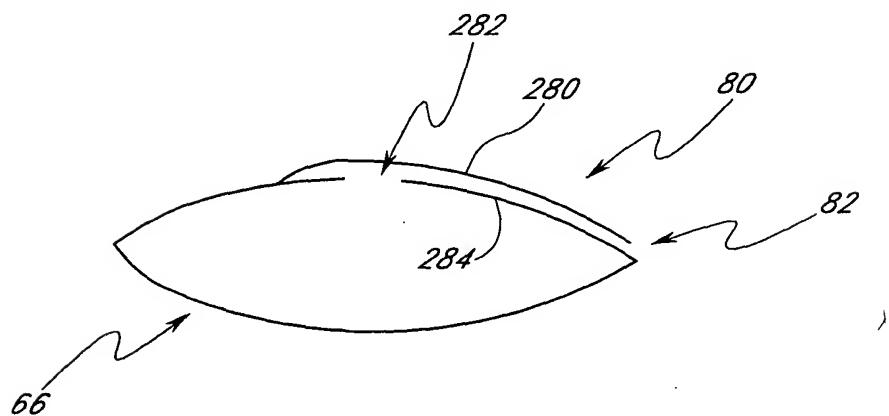


FIG. 37

HIGH VAPOR PRESSURE ATTENUATION DEVICE

Kevin G. Connors et al.

Appl. No.: Unknown Atty Docket: SOLACE.4CP1C4

38/4.7

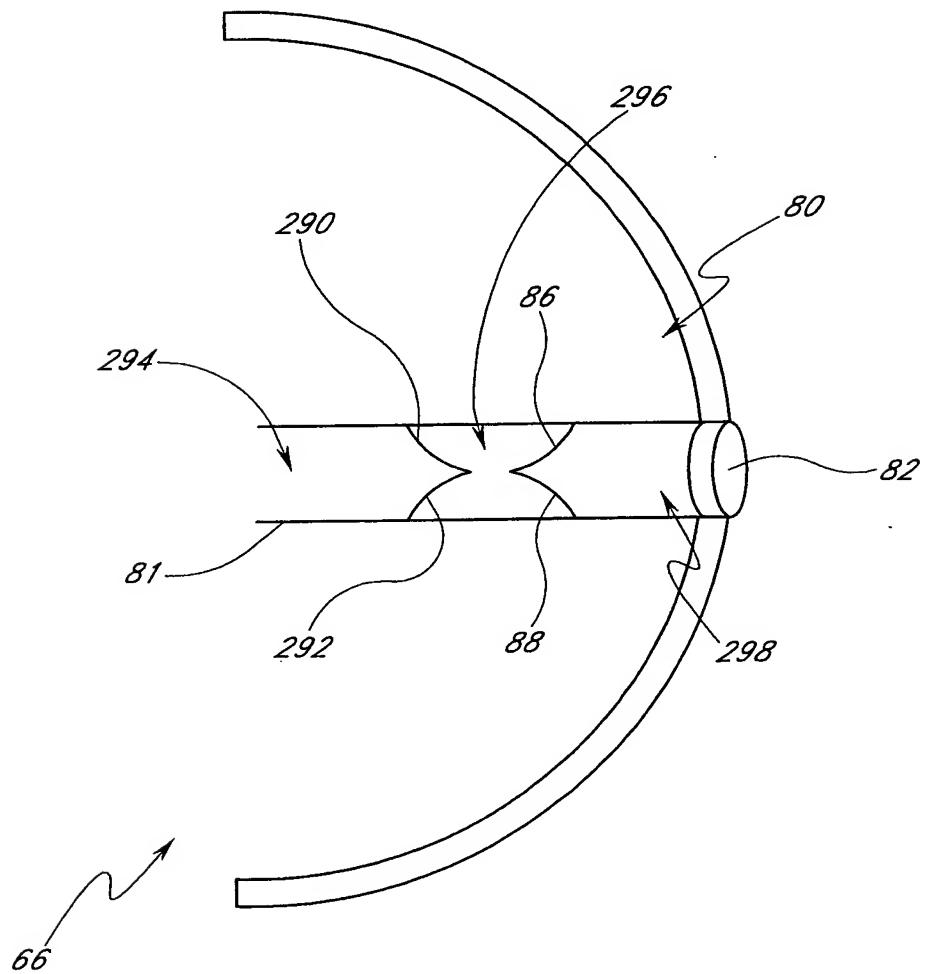


FIG. 38

FIG. 39A

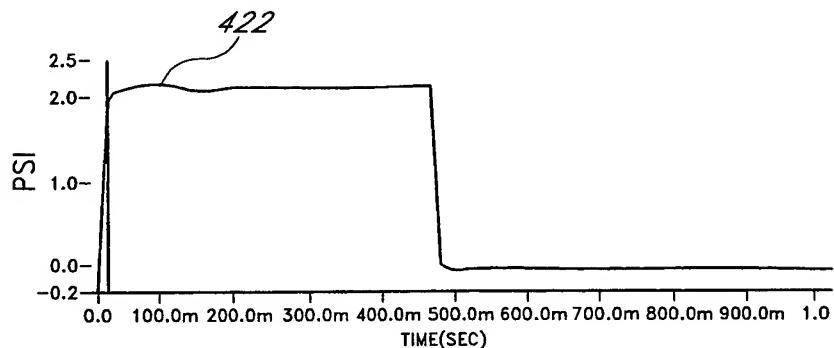


FIG. 39B

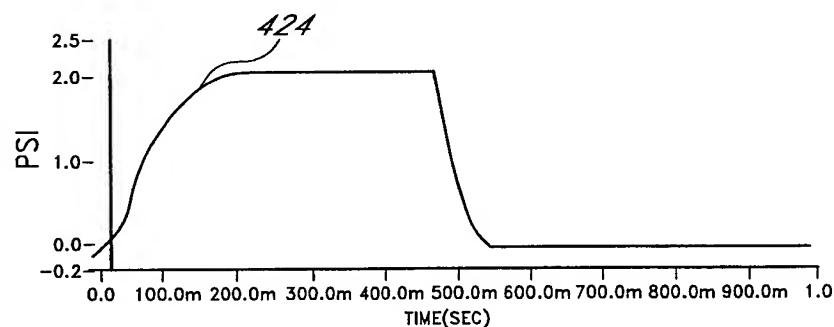


FIG. 39C

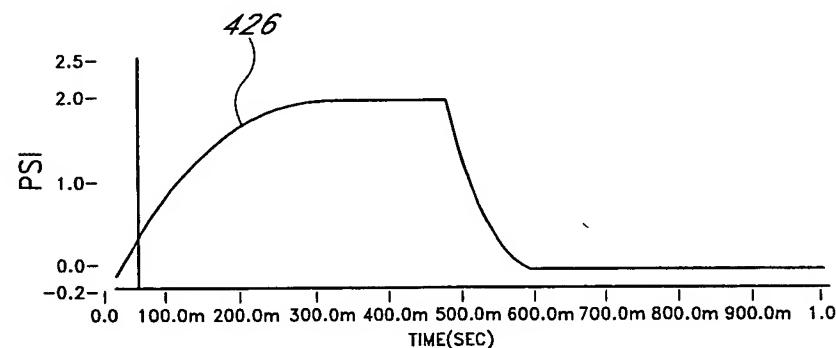


FIG. 39D

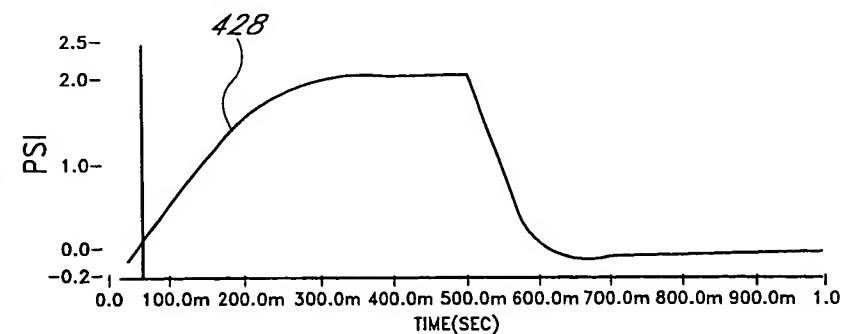


FIG. 40A

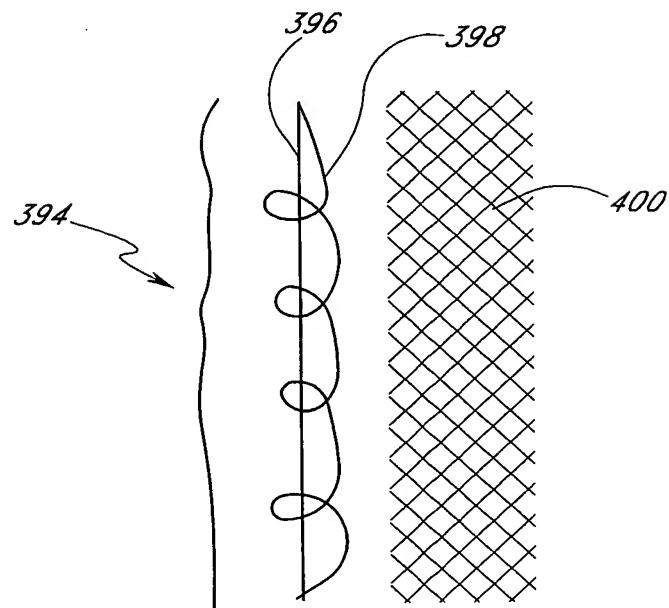
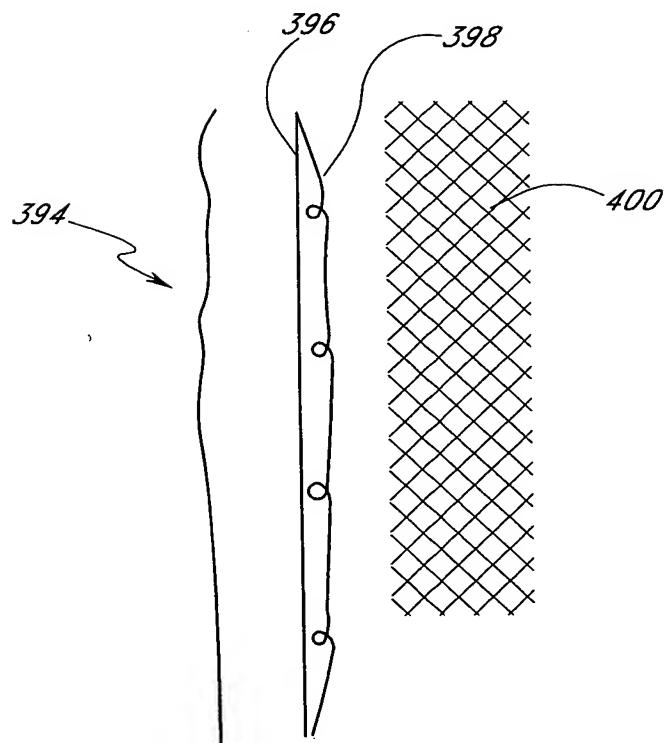


FIG. 40B



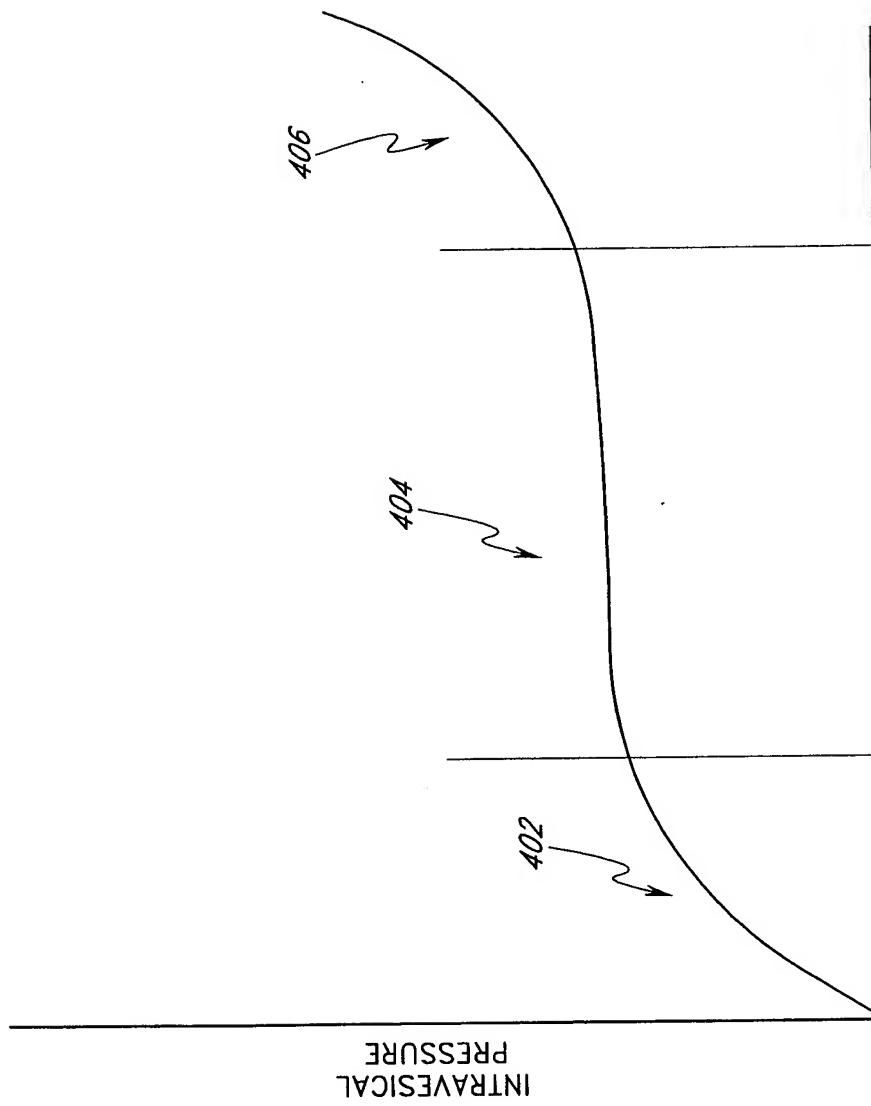


FIG. 41

INTRAVESICAL
PRESSURE

HIGH VAPOR PRESSURE ATTENUATION DEVICE
Kevin G. Connors et al.
Appl. No.: Unknown Atty Docket: SOLACE.4CP1C4

42/47

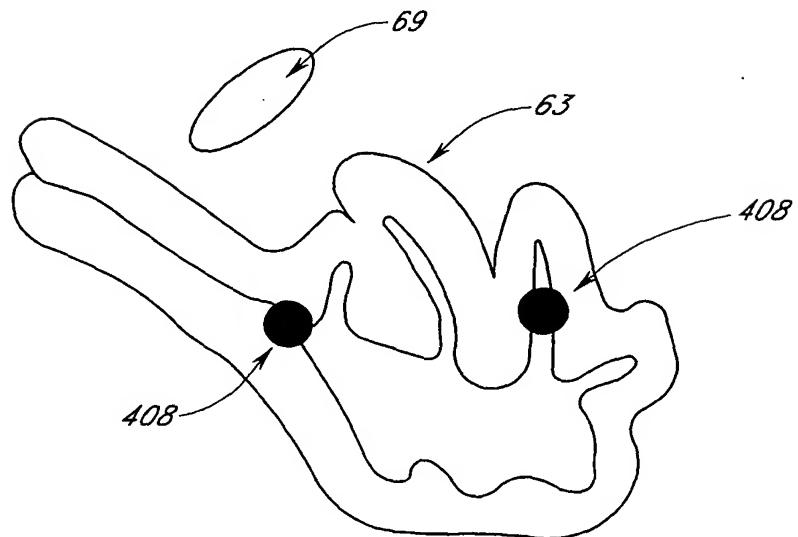


FIG. 42

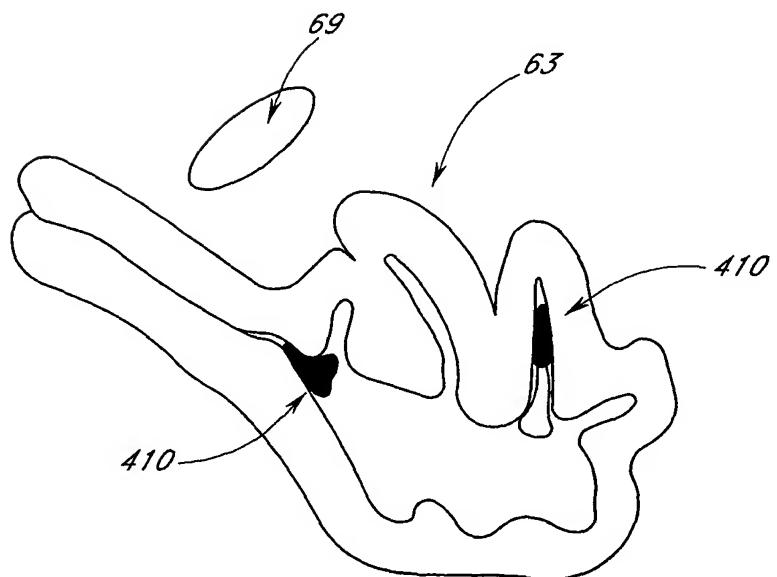


FIG. 43

FIG. 44A

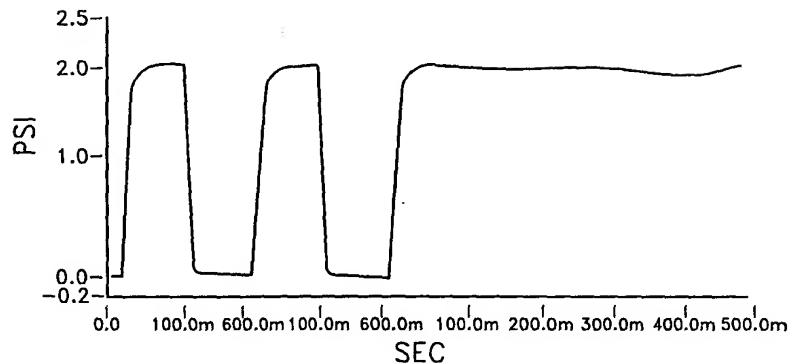


FIG. 44B

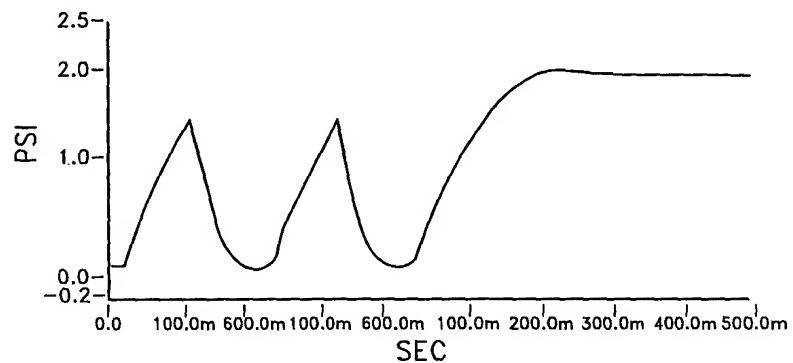


FIG. 44C


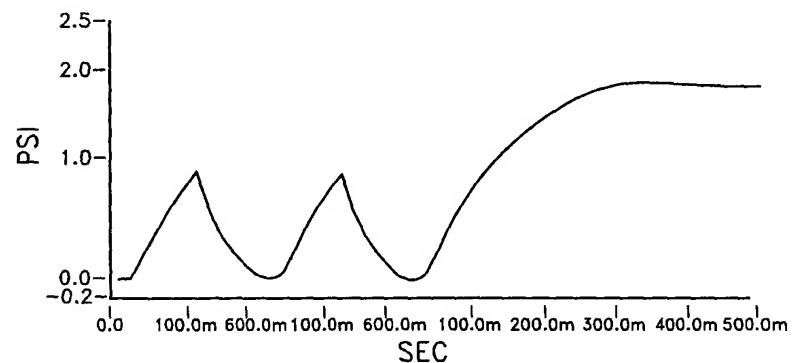


FIG. 44D

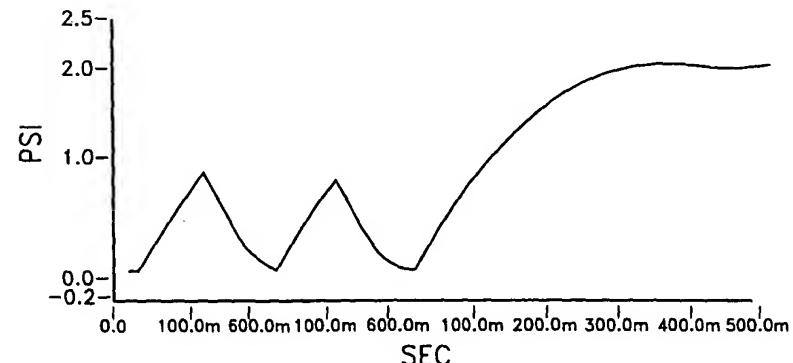

HIGH VAPOR PRESSURE ATTENUATION DEVICE

Kevin G. Connors et al.

Appl. No.: Unknown Atty Docket: SOLACE.4CPI C4

44/47

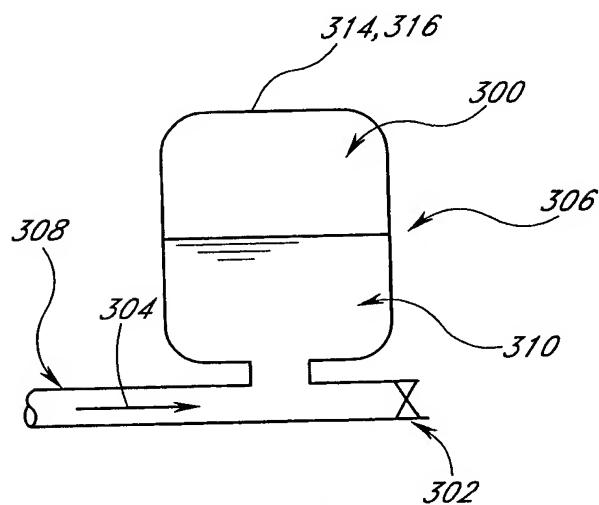


FIG. 45

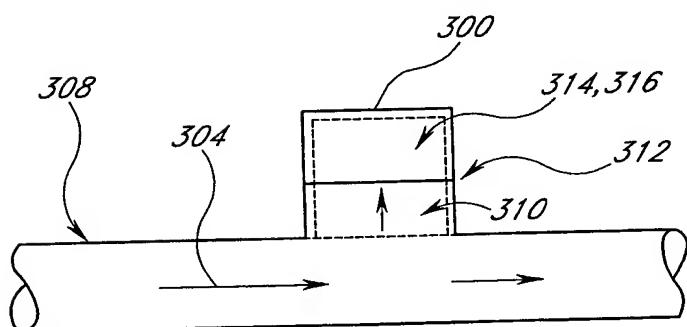


FIG. 46

HIGH VAPOR PRESSURE ATTENUATION DEVICE
Kevin G. Connors et al.
Appl. No.: Unknown Atty Docket: SOLACE.4CP1C4

45/47

FIG. 47 A

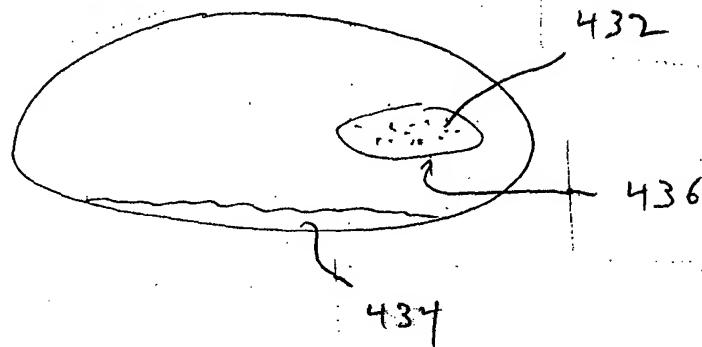


FIG. 47 B


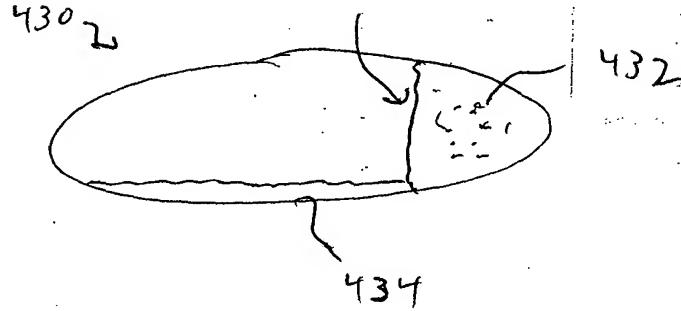


FIG. 47 C

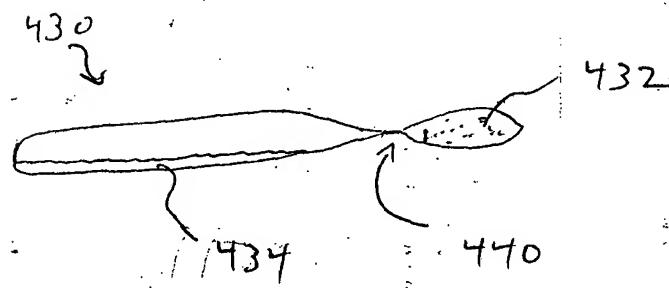

HIGH VAPOR PRESSURE ATTENUATION DEVICE
Kevin G. Connors et al.
Appl. No.: Unknown Atty Docket: SOLACE.4CP1C4

FIG. 48 A

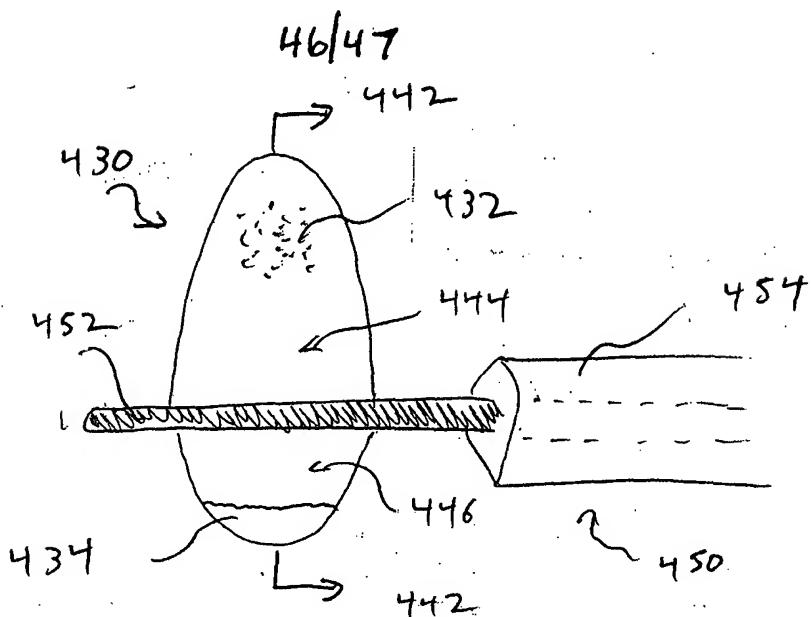


FIG. 48 B

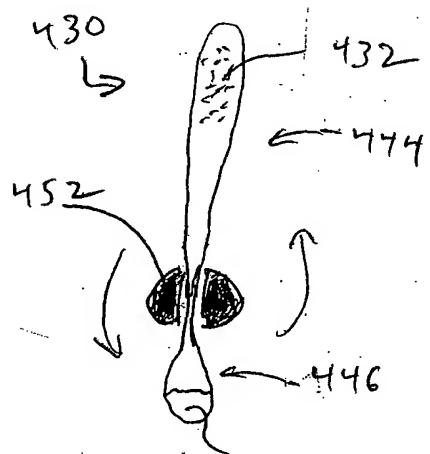


FIG. 48 C

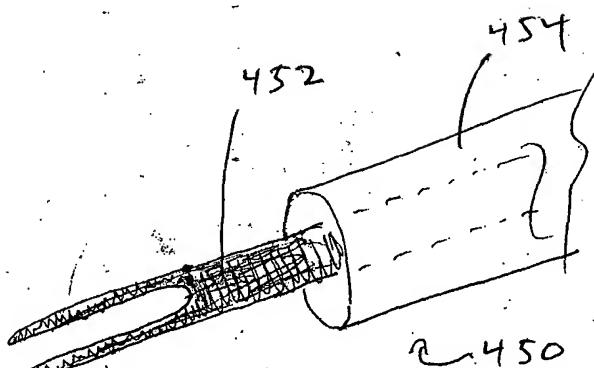


FIG. 48 D

47/47

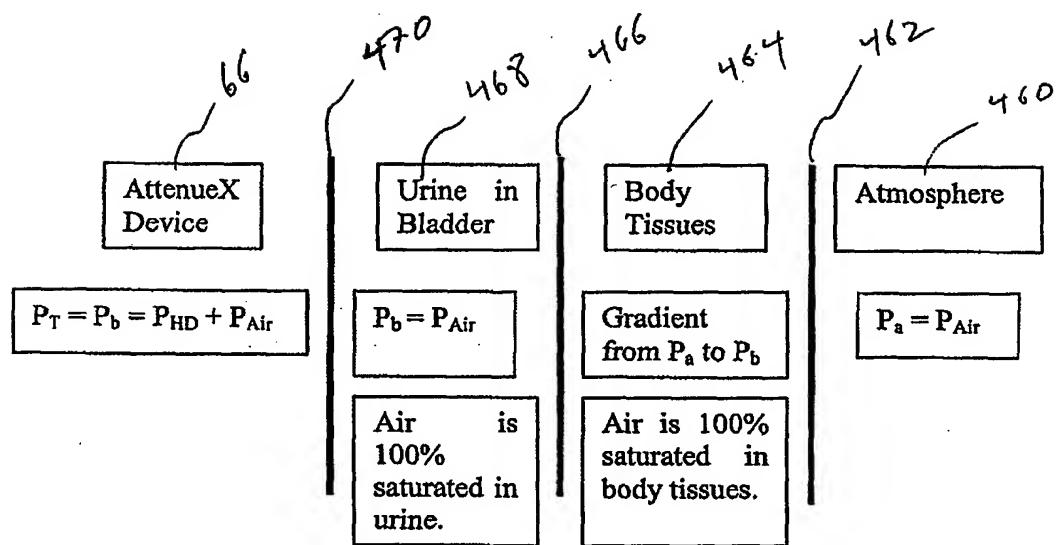


FIG. 49